


Author Query Form

Reviewer 4 - 2nd round

AQ1. Figure 1 should show the workflow of an AR-enabled system, not an HMD device. The author needs show to help the reader understand the working process of AR in a surgical system.

R1: We would like to thank the Reviewer for this suggestion. We realized the following scheme in order to make the article clearer.

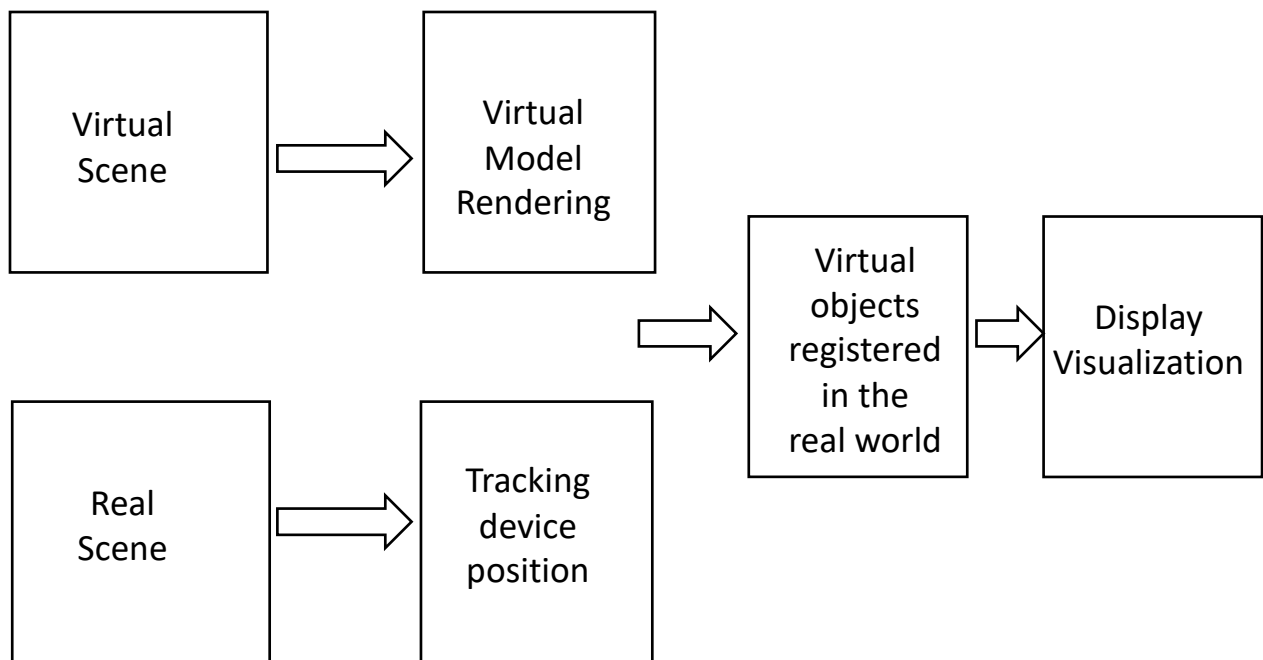

AQ2. Figures 5, 6, and 7 are actually Tables, please reproduce accordingly.

R2: As suggested by the Reviewer we proceeded to substitute “Figure” with “Table” in the mentioned cases.