

Review

Expert System and Decision Support System for Electrocardiogram Interpretation and Diagnosis: Review, Challenges and Research Directions

Kayode S. Adewole ¹, Hammed A. Mojeed ¹, James A. Ogunmodede ², Lubna A. Gabralla ³, Nasir Faruk ⁴, Abubakar Abdulkarim ⁵, Ifada Emmanuel ⁴, Yusuf Y. Folawiyo ⁴, Abdulkareem A. Oloyede ⁴, Lukman A. Olawoyin ⁴, Ismaeel A. Sikiru ⁶, Musa Nehemiah ⁷, Abdulsalam Ya'u Gital ⁷, Haruna Chiroma ^{8,*}

¹ Department of Computer Science, University of Ilorin, Nigeria; adewole.ks@unilorin.edu.ng, mojeed.ha@unilorin.edu.ng

² Department of Medicine, University of Ilorin, Nigeria; ogunmodede.ja@unilorin.edu.ng

³ Department of Computer Science and Information technology, Applied College, Princess Nourah Bint Abdulrahman University, P.O. Box 84428, Riyadh 11671, Saudi Arabia; lubnagabralla@gmail.com

⁴ Sule Lamido University, Kafin Hausa, Nigeria; nasirfaruk@gmail.com, emmanuelifada7@gmail.com, yusuf-folawiyoyusuf@gmail.com, oloyede.aa@unilron.edu.ng, lolawoyin@gmail.com

⁵ Department of Electrical & Electronics Engineering, Ahmadu Bello University Zaria, Nigeria; abdulkarima@abu.edu.ng

⁶ Department of Information and Communication Science, University of Ilorin, Nigeria; idhikrullah@gmail.com

⁷ Department of Mathematical Sciences, Abubakar Tafawa Balewa University, Bauchi, Nigeria; nehemiahmusa7@gmail.com, asgital@gmail.com

⁸ University of Hafr Al-Batin, College of Computer Science and Engineering, Saudi Arabia; charuna@uhb.edu.sa

* Correspondence: charuna@uhb.edu.sa

Abstract: Electrocardiography (ECG) is one of the most widely used recordings in clinical medicine. ECG deals with the recording of electrical activity that is generated by the heart through the surface of the body. The electrical activity generated by the heart is measured using electrodes that are attached to the body surface. The use of ECG in the diagnosis and management of cardiovascular disease (CVD) has been in existence for over a decade, and research in this domain has recently attracted large attention. Along this line, an expert system (ES) and decision support system (DSS) have been developed for ECG interpretation and diagnosis. However, despite the availability of large literature, access to recent and more comprehensive review papers on this subject is still a challenge. This paper presents a comprehensive review of the application of ES and DSS for ECG interpretation and diagnosis. Researchers have proposed a number of features and methods for ES and DSS development that can be used to monitor a patient's health condition through ECG recordings. In this paper, a taxonomy of the features and methods for ECG interpretation and diagnosis have been presented. The significance of the features and methods, as well as their limitations, were analyzed. The review further presents interesting theoretical concepts in this domain as well as identifies challenges and open research issues on ES and DSS development for ECG interpretation and diagnosis that require substantial research effort. In conclusion, this paper identifies important future research areas with the purpose of advancing the development of ES and DSS for ECG interpretation and diagnosis.

Keywords: Electrocardiogram; ECG; Cardiovascular disease; Expert system, Decision support system; Heartbeat; Heart rate variability.

Citation: To be added by editorial staff during production.

Academic Editor: Firstname Last-name

Received: date

Accepted: date

Published: date

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

1. Introduction

The Electrocardiography (ECG) is one of the most widely used recordings in clinical medicine. ECG involves the recording of electrical activity that is generated by the heart through the surface of the body. Historically, the first ECG recording was dated back to 1887 [1]. The electrical activity generated by the heart is measured using electrodes placed on specific parts of the body surface. ECG devices are typically used to obtain information about the physiological condition of the heart by measuring the electrical signals generated by the heart through electrodes attached non-invasively to the body surface [2]. Single-lead three-electrodes ECG recordings have been widely used [3, 4]. However, due to the advancement in research, the number of leads has gradually increased to obtain a more accurate ECG recording [5, 6]. An ECG recording is one of the most valuable data used in diagnosing heart disease. It offers unique information that is not obtainable from any other type of test. Even though ECG signal is widely recorded in hospitals, it is also used in epidemiological studies as well as in large clinical trials [4, 5, 7].

One technique commonly used in epidemiological studies for classifying ECG is known as the Minnesota coding, whereby an internationally agreed set of rules is used to describe the ECG patterns [8]. This is particularly favoured by epidemiologists in large-scale population studies. Currently, sensors can be used to automatically measure ECG signals instead of the conventional discrete measurement [4, 5, 8, 9]. Automated techniques for Minnesota coding are available and are valuable when a large numbers of ECGs require coding. Recently, computer analysis of the ECG was developed for recording and interpreting ECGs. This helps in developing ECG data repositories and reducing the time lag in ECG reports. Besides ECG signals, other forms of real-time biomedical signals have been collected from the human body, which include blood pressure, respiration rate, heart rate, blood glucose, galvanic skin response and oxygen saturation levels among others. The list of collectable physiological signals is rapidly expanding owing to the speed of on-going technological advancements in biomedical domain [10, 11]. These signals, especially the ECG, have helped in detecting and diagnosing various types of diseases, including cardiovascular diseases (CVD).

CVD is a group of diseases that involves the heart and/or blood vessels [12]. CVD includes coronary artery diseases (CAD) such as angina and myocardial infarction (heart attack), heart failure, stroke, hypertensive heart disease, rheumatic heart disease, cardiomyopathy, heart arrhythmia, congenital heart disease, valvular heart disease, carditis, aortic aneurysms, peripheral artery disease, thromboembolic disease and venous thrombosis among others [12]. CVD is the leading global cause of death and accounts for 17.3 million deaths per year. This number is estimated to increase and reach about 23.6 million by 2030 [13, 14]. According to World Health Organization (WHO), 17.7 million people died from CVD in 2015, representing 31% of all global deaths and about half of total deaths from Non Communicable Diseases (NCD). Out of the 17.7 million, an estimated 7.4 million were caused by CAD and 6.7 million were caused by stroke. Increasingly, the population mostly affected are those in low and middle-income countries, where about 80% of these deaths occurred at younger ages [13, 15, 16]. To predict the occurrence of CVD such as heart arrhythmia, an ECG is generally used by doctors to identify the condition in patients. However, widespread recognition and early prevention of such diseases is a challenge due to the shortage of cardiologists who are proficient in ECG interpretation and affordability of ECG equipment. Hence, automated analysis and classification of CVD are expected to play a significant role in accurately detecting the abnormalities of the heart in advance [17]. CVD diagnosis from ECG has significant importance in the biomedical domain. As reported in the medical literature, the two widely known heart diseases are cardiac arrhythmias and myocardial ischaemia. Myocardial ischaemia occurs due to the shortage of blood supply to the myocardium, which affects the morphology of the heart ECG signal. Conversely, cardiac arrhythmias indicate abnormalities in the rhythm of the heart, which may lead to cardiac arrest, chest pain or



sudden cardiac death [18]. For effective diagnosis of CVD using ECG signal data, several expert system (ES) and decision support system (DSS) have been developed.

ES is a problem-solving system which can produce better performance in a specialized problem area that typically requires expert knowledge and skills. ES program processes the knowledge of experts to mimic their skills, thinking and perception [19]. ECG data collected from the sensors can be transferred to a cloud server to conduct a preliminary automatic diagnosis based on the knowledge base of the ES without the presence of medical experts [4, 20]. A knowledge base is initially developed using a large sample dataset, which can be updated frequently by specialists to improve the accuracy of the ES and DSS for disease prediction [4]. Such ES and DSS systems will assist patients to detect abnormalities in their heart before seeing their doctor or physicians for treatment [2, 4, 5].

In this paper, a comprehensive review of existing state-of-the-art studies on ES and DSS for ECG interpretation and diagnosis is presented. To avoid duplication of the review, we conducted a wide range of literature searches from reputable databases to identify any existing review articles on ES and DSS specifically for ECG interpretation and diagnosis. Indeed, there have been review studies on related topics. The most recent of these studies are the review articles by [16], [21] and [22] published in IEEE Xplore, PubMed and ScienceDirect respectively. Gahlot, Reddy [16] presents a survey of smart health monitoring approaches by considering different parameters such as framework, targeted population, monitoring device, processor utilized, integrated sensors, and communication module. The review summarized different technologies implemented for health monitoring towards making the healthcare domain smarter. They outlined smart and traditional monitoring systems by categorizing them as a mobile, wearable, and remote health monitoring systems. The authors present challenges hindering such system development. To understand the real-time societal need of this smart healthcare system, a survey questionnaire was conducted targeting 183 valid-independent entries collected from various regions. The study concluded that there is a need for developing an integrated platform to achieve comprehensive healthcare monitoring system that is adaptable to different situations. Li, White [21] conducted a narrative review on a number of mobile phone apps that are capable of monitoring atrial fibrillation (AF), heart rate (HR), and heart rate variability (HRV). The authors searched PubMed and EMBASE databases until October 2018 for relevant articles on the subject. They observed that the operation of the mobile apps involved the use of either a photoplethysmographic recording or a handheld external electrocardiographic recording device connected to the mobile phone or wristband. The authors concluded that mobile phone apps have a significant roles to play in the screening, diagnosis, and monitoring of arrhythmias and HR. Rong, Mendez [22] investigated the application of Artificial intelligence (AI) in the biomedical domain. The authors summarized the latest developments of applications of AI in the biomedical fields, including disease diagnosis, living assistance, biomedical information processing, and investigation. The review considered 20 years literature from 1999 to 2018 and concluded that the application of AI in biomedicine is still in its infantile stage. Two case studies were explored to demonstrate the prediction of epileptic seizure occurrence and the filling of a dysfunctional urinary bladder. However, Rong, Mendez [22] review article does not provide a detailed discussion on the application of ES and DSS with a specific focus on ECG interpretation and diagnosis.

This paper provides a comprehensive review of the state-of-the-art methodologies for the development of ES and DSS systems targeted to ECG interpretation and diagnosis. We propose taxonomies of features and methods that have been utilized to interpret ECG signals. Our review covered a wide range of reputable databases including, IEEE, PubMed, ScienceDirect, Springer, Wiley, and ACM. In addition, this paper presents the challenges and open research issues that are worthy of exploration towards the development an efficient ES and DSS system for ECG interpretation and diagnosis. A total of 85 articles have been considered after a thorough screening of the available literature in the target subject based on the guidelines of Preferred Reporting Items for Systematic

Reviews and Meta-Analyses (PRISMA) [23]. These articles covered over a decade from 2010 to 2020. We focused on the recent developments and advances as highlighted in the reviewed articles.

The remaining part of this paper is organized as follows: Section 2 presents the review methodology employed in this study. It discusses the inclusion and exclusion criteria used to select the relevant articles for the study. Section 3 presents an extensive discussion on ECG. Section 4 highlights the composition of ES and DSS systems designed to aid ECG acquisition and interpretation. Section 5 focuses on the mobile applications for ECG data acquisition and interpretation. Section 6 presents a taxonomy of methods for ES development, specifically for ECG. Section 7 discusses the taxonomy of the various features that have been used for ECG interpretation. Section 8 highlights a number of contemporary research issues and presents future research directions in DSS development for ECG interpretation and diagnosis.

2. Review Methodology

The This study employed the guideline proposed by PRISMA to select relevant articles for the study. PRISMA provides comprehensive guidelines for reporting systematic review and meta-analyses studies using evidence-based minimum set of items [23]. This review considered publications that focused on ECG interpretation and diagnosis, a mobile applications or frameworks for ECG interpretation, as well as studies on ES and DSS for ECG interpretation and diagnosis. These publications were retrieved through a careful literature search using reputable high-impact research databases such as IEEE, PubMed, ScienceDirect, Springer, Wiley and ACM. The following query set was used to retrieve the relevant publications:

("mobile application" OR "framework") AND ("ECG" OR "ECG tracing" OR "electrocardiogram") AND ("expert system" OR "decision support system")

This query set retrieved a total record of 8,370 publications which were passed to the screen phase of the model. By following PRISMA guidelines, the titles and abstracts of the total articles retrieved were thoroughly screened for relevance. The eligibility criteria were based on the relevance of the articles using the major keywords employed in the search query. After careful consideration of the inclusion and exclusion criteria, a total of 85 studies were considered for review. Figure 1 shows the flow chart of the study selection based on PRISMA guidelines.

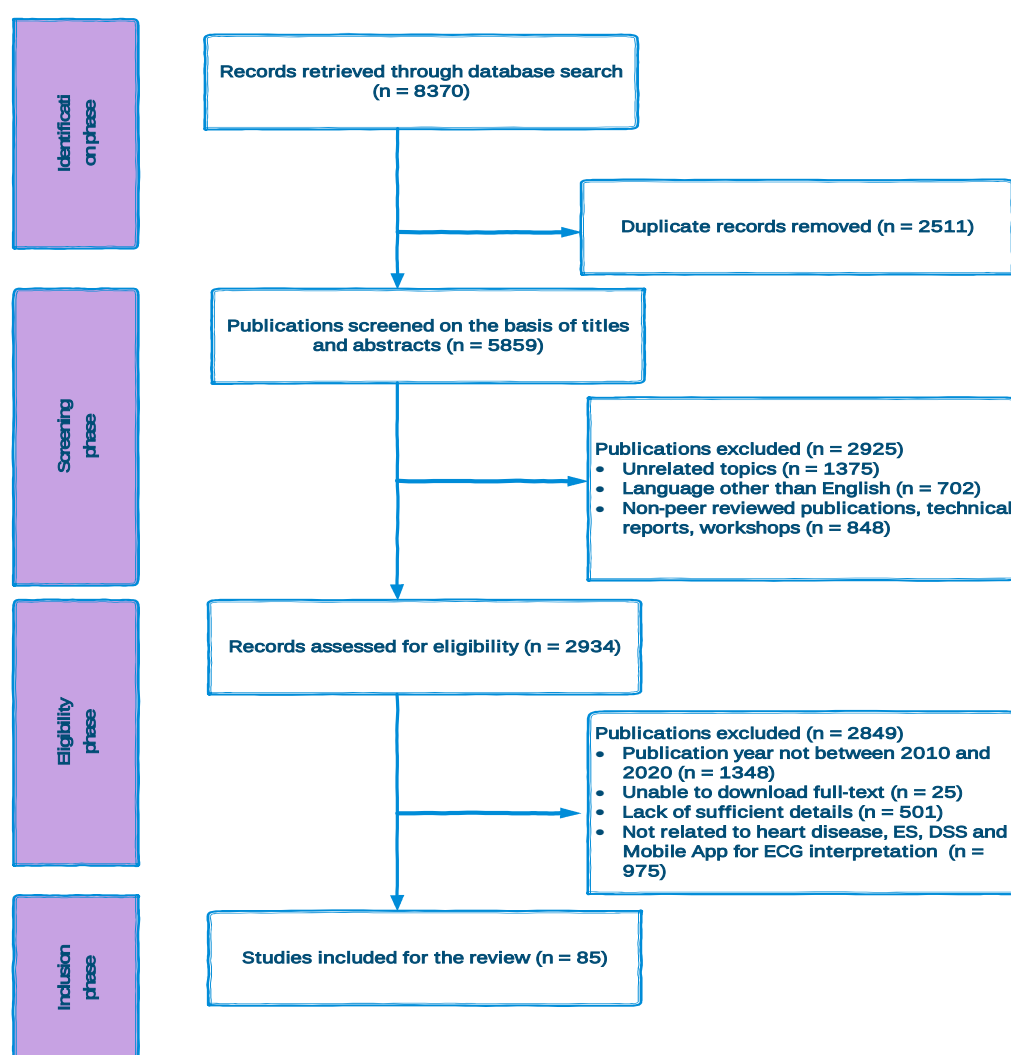


Figure 1. Study selection flow chart based on PRISMA model

The included studies in the review covered over a decade which spanned eleven-year period from 2010 to 2020. More specifically, we focused on publications written in English language. Table 1 summarizes the studies considered in this review. Interestingly, research on ES and DSS for ECG interpretation and diagnosis has witnessed tremendous growth over the past few years. Researchers have investigated and explored the possible use of mobile application development to reduce the stress in ECG data acquisition and diagnosis [24–27]. Cloud-based model [4, 14], ontology framework [28, 29], wearable sensors [10, 30], XML rule-based repository [31] as well as Internet-of-Things (IoT) [4] among others have been considered to aid in the diagnosis of heart diseases. Recent research effort has been directed towards developing solutions for securing ECG data based on biometric authentication [6, 32]. There have been a significant number of studies on arrhythmia detection and diagnosis [17, 33–35]. The subsequent sections detailed the efficacy of research efforts in ECG interpretation and diagnosis. Figure 2 shows the percentage distribution of the publications considered in this review. This distribution is to ensure that recent studies are critically examined while at the same time exploring the research trend in the domain of ES and DSS for ECG interpretation and diagnosis.

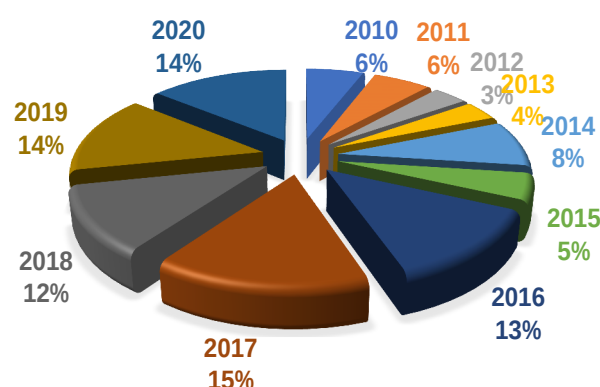


Figure 2. Percentage distribution of the studies per year

Table 1. Summary of the studies considered in this review

S/No	Author	Year	Objective	Methodology
1	Bellos, Papadopoulos [30]	2010	To develop a system that estimates the severity of a health episode of patients by collecting and analyzing patient information for disease using wearable sensors.	Fiducial features and ANN
2	Bond, Finlay [31]	2010	To design an approach to interpretXML the ECG recording of patients based on ECG Rule Markup Language(ecgRuleML) to externalize decision rules.	knowledge-based
3	Minutolo, Sannino [28]	2010	To develop a mobile mHealth system to attend to abnormal or emergency for patients suffering from heart problem	Ontology
4	Catley, Smith [36]	2010	To propose a framework that can be used for supporting complex real-time ECG analysis based on clinical rules translation models	Data streaming
5	Mahmoodabadi, Ahmadian [37]	2010	To design an expert system for ECG heart arrhythmia detection	Fiducial and Discrete Wavelet Transform
6	Karvounis, Katertsidis [38]	2011	To present the Specialist's Decision Support System (SDSS) for disease diagnosis	Framework
7	Kopiec and Martyna [39]	2011	To use the SVM Machine LearningSVD, Haar wavelet, algorithm for ECG classification and detection of QRS-complexes, P- and T-waves in the 12-lead ECGSVM	Discrete Fourier Transform and

			signal.	
8	Abdullah, Zakaria [40]	2011	To predict the hypertension risk of patients using Fuzzy Expert System	Fuzzy-based approach
9	Bellos, Papadopoulos [27]	2011	To design procedures for diagnosing and monitoring chronic heart disease patient remotely	Machine learning using SVM, Random Forests, Artificial Neural Networks, Decision Trees and Naïve Bayes
10	de Oliveira, Andreão [41]	2011	To apply Bayesian Networks to detect cardiac arrhythmias	Bayesian Network
11	Acampora, Lee [42]	2012	To design an ECG based decision support system for predicting cardiac quality level	Ontology and Fuzzy-based approach
12	Cinaglia, Tradigo [43]	2012	The develop a mobile system for telecardiology investigations	Framework
13	Sahin, Tolun [44]	2012	To analyze various hybrid expert system approaches and their applications	Review paper
14	Paliwal and Kiwelekar [45]	2013	To identify similarities and variabilities among existing MPMs	Body Area Network (BAN) and Back-End Systems (BESys).
15	Belle, Kon [46]	2013	To carry out a survey of applications and methodologies for designing computer aided Decision Support System in biomedical informatics	Review paper
16	Lin, Labeau [47]	2013	The study presents a design of a telecommunication and computer-based system for monitoring patients in comorbid condition	Logical model-based algorithms
17	Prerana, Cheeran [48]	2014	To develop a mobile android application prototype that is compatible with existing ECG acquisition device for ECG analysis	Fiducial
18	Benharref, Serhani [9]	2014	To develop a smart and adaptive	Cost-oriented

			synchronization model for m-Health applications	algorithms
19	Lin and Labeau [49]	2014	To design and implement a decision support system for monitoring patients with critical conditions	
20	Martínez-Pérez, de la Torre-Díez [50]	2014	To investigate existing mobile application for medical decision support	Review paper
21	Sani, Islam [51]	2014	To propose a framework for remote diagnosis and monitoring of heart attack ambulatory patient	Rule-based
22	Tanantong, Nantajeewarawat [52]	2014	To develop a hybrid continuous cardiac monitoring framework for false alarm reduction	Machine learning and rule-based ES
23	Thomas, Das [53]	2014	Develop a dual tree complex wavelet transform based framework for ECG feature extraction	Fiducial and dual tree complex wavelet transform
24	Sterling, Huang [54]	2015	To develop a novel machine learning classification approach to analyze the electrocardiogram of atrial fibrillation patients	MP features and quadratic discriminant analysis-based classification
25	Alshraideh, Otoom [55]	2015	Aim to apply data mining techniques for identifying individuals suffering from heart arrhythmias.	Machine learning algorithms such as C 4.5, NN, SVM, Jrip and Naïve bayes
26	Amour, Hersi [25]	2015	Propose an ECG system to remotely monitor multiple patients with cardiovascular diseases	Fiducial
27	Prakash [56]	2015	To develop an intelligent clinical decision support system for diagnosing heart disease	Case-Based Reasoning
28	Cloughley, Bond [57]	2016	To construct an ECG interpretation of clinical decision support tool	Fiducial and SQL query
29	Desai, Martis [58]	2016	To investigate and evaluate the performance of selected three feature extraction methods for	DCT, DWT, PCA, ANOVA, and k-NN

			ECG arrhythmia classification	
30	Alickovic and Subasi [34]	2016	To design an automatic detection and classification model for arrhythmia	DWT and Random Forests classifier
31	Li, Wang [59]	2016	To detect attenuating frequencies of the ECG signal related to artifacts	Wavelet packet entropy and random forests
32	Ripoll, Wojdel [60]	2016	To develop an automatic screening method for predicting the need for ambulatory patient to require cardiology service	Deep neural networks
33	Jeyalakshmi and Robin [61]	2016	To analyse Heart Rate Variability in diagnosing of sleep apnea	Fuzzy-based
34	Kotevski, Koceska [62]	2016	To develop an e-health system for monitoring of vital physiological data of patients	Open m-Health platform
35	Baheti [63]	2016	The paper gives a guide for applying fuzzy logic approach in developing expert system for varieties of diseases in India	Fuzzy-based
36	Hassan and Bhuiyan [64]	2016	Propose splitting of EEG signals into wavelet subbands using tunable output factor and spectral characteristics	Tunable-Q factor wavelet transform and Random forest
37	Li, Wang [59]	2016	To develop a personalized automatic machine learning model heartbeat classification	Parallel general regression neural network
38	Hejazi, Al-Haddad [65]	2016	To develop ECG biometric authentication using kernel approach for ECG tracing	Non-fiducial with Kernel-based
39	Gharehbaghi, Lindén, & Babic (2017)	2017	Propose machine learning method for developing decision support system for cardiac disease diagnosis	Hidden markov model
40	Desai [67]	2017	To design an automated classification of normal and Coronary Artery Disease conditions of ECG	DWT, DCT, PCA and k-NN, SVM
41	Domazet, Gusev [26]	2017	To provide design specifications for time-critical medical monitoring applications	Framework
42	Thai, Minh [4]	2017	To developed a IoT mechanism for	Revised Sequential

			automatically extract information related to heart disease from filtered ECG signals	Recursive algorithm, DWT and Fishers Linear Discriminant
43	Yin and Jha [10]	2017	To present HDSS, a closed-loop multitier health decision support system	Ensemble approach
44	Hassan and Haque [68]	2017	To develop a wearable low-power sleep apnea monitoring device for in-home care	Tunable-Q factor wavelet transforms and RUSBoost classifier
45	Zhang, Wang [69]	2017	To improve the classification performance of ECG diagnosis algorithm	Recurrent neural networks (RNN) and density-based clustering technique
46	Hossain, Mirza [70]	2017	Utilizing the power of crowdsourcing to minimize the response time and cost of operating emergency medical service	Crowdsourcing method
47	Cairns, Bond [71]	2017	Improving accuracy of interpretations of the 12-lead ECG and to minimize missed co-abnormalities	Differential Diagnoses Algorithm
48	Sadrawi, Lin [35]	2017	The study evaluates the performance of four datasets from PhysioNet physiological repository	Periodogram approach for VF detection
49	Krasteva, Jekova [72]	2017	Proposed cross-correlation analysis of 12-lead ECG signals	Non-fiducial using Cross-correlation analysis
50	Jung and Lee [73]	2017	Propose ECG identification method based on non-fiducial feature extraction and window removal method	Window removal method for feature extraction. Nearest neighbor (NN), support vector machine (SVM), and linear discriminant analysis (LDA) for classification.

51	Hejazi, Al-Haddad [74]	2017	To develop ECG biometric authentication system based on non-fiducial autocorrelation method	Non-fiducial autocorrelation and kernel-based method and one-class SVM
52	Gahlot, Reddy [16]	2018	To review smart health monitoring approaches	Review paper
53	Venkatesan, Karthigaikumar [18]	2018	To improve classification of arrhythmia detection system	DENLMS adaptive filter, Coiflet wavelet, HRV features and SVM
54	Wang, Sun [14]	2018	To analyze telemonitoring of health care based on intelligent analysis of unstructured big data in real-time.	Big data
55	Yang, Si [17]	2018	To improve the ECG classification speed by applying principal component analysis network (PCANet) for feature extraction on a noisy ECG signal.	PCANet and SVM
56	Jangra and Gupta [75]	2018	To develop real-time patient supervision system using IoT-based smart monitoring model.	Internet-of-things framework
57	Plawiak [76]	2018	To create new and efficient methods for automated detection of myocardial dysfunctions	Machine learning using SVM, k-NN, PNN, and RBFNN
58	Kumar, Pachori [77]	2018	To propose a automatic approach for the diagnosis of AF patients	entropy-based features in flexible analytic wavelet transform (FAWT)
59	Arteaga-Falconi, Al Osman [78]	2018	To develop biomodal authentication system by fusing ECG and fingerprint features	Non-fiducial using Morphological-based approach
60	Arteaga-Falconi, Al Osman [78]	2018	Proposed continuous authentication scheme based on ECG streams for real-time authentication	Non-fiducial using ECG streams method
61	Lee, Jeong [79]	2018	To propose effective method for fiducial points detection from ECG signal	Polygonal approximation
62	Comito, Forestiero [80]	2019	To implements a set of services to	Deep learning

			support physicians in diagnosing or treating patients health issues	
63	Chauhan, Vig [81]	2019	To automatically detect the anomalous cardiac events directly from machine-readable, recorded ECG signals	Machine learning such as Multilayer perceptron, SVM and logistic regression.
64	Goshvarpour and Goshvarpour [6]	2019	To develop an ECG-based automated human identification system	Fiducial and non-fiducial based methods. Information gain ratio and k-NN.
65	Abdalla, Wu [33]	2019	To target effective method for arrhythmia detection and classification	Nonlinear and nonstationary decomposition method
66	Jain and Kaur [82]	2019	To design a fuzzy expert system for the diagnosis of coronary artery heart disease.	Fuzzy-based approach
67	Sharma, Madaan [83]	2019	To design an expert system to predict heart disease using Fuzzy approach	Fuzzy-based approach
68	Goshvarpour and Goshvarpour [6]	2019	The study focuses on low accuracy ECG-based system for security purpose	Information theory
69	Mincholé and Rodriguez [84]	2019	To apply deep learning algorithm for identification of normal and abnormal heart rhythms	Deep learning
70	Kaleem and Kokate [85]	2019	To develop an efficient, flexible filtering technique to remove the heartbeat signal	Adaptive Filtering and Artificial neural network
71	Jovic, Kukolja [86]	2019	The study presents MULTivariate Time Series Analysis in Biomedicine (MULTISAB) system	Multithread parallelization approach
72	Khatibi and Rabinezhadsadatmahaleh [87]	2019	To automatically classify ECG beats for arrhythmia detection	Deep learning, k-NN, SVM and Random forest
73	Li, White [21]	2019	To investigate and review the current state of mobile phone applications in cardiac Arrhythmology	Review paper
74	Zarei and Asl [3]	2020	To introduce new features for the	Machine learning

			classification of sleep apnea and normal parients	using GentleBoost classifier
75	Rong, Mendez [22]	2020	To study the new scientific applications of AI in biomedicine	Review paper
76	Akhtar, Lee [88]	2020	To present state-of-the-art Big Data analytics tools	Review paper
77	Christo, Nehemiah [89]	2020	To apply optimization of tree based classifier for heart disease diagnoses	Co-operative Co-evolution and Random Forest
78	Subasi, Bandic [90]	2020	To develop intelligent cloud-based system with wearable biomedical sensors to predict chronic disorders in a real time	Machine learning algorithms
79	Parekh, Shah [91]	2020	To give significant detection methods and systematic approaches to figure out the impacts and causes of fatigue	Machine learning using ANN
80	Santra, Basu [92]	2020	To develop a rough set-based lattice framework to address the problem of redundancy and inconsistency in ECG knowledge discovery	Rough set-based lattice structure
81	Kar, Sahu [93]	2020	To develop effective DSS for ECG signals analysis and arrhythmia detection	Dual-tree complex wavelet transform
82	Bhatt, Dubey [94]	2020	To model a framework that can help avoid sudden cardiac arrest and sudden cardiac death	Framework
83	Hosseini, Tran [95]	2020	To develop an autonomic brain computing system for localization and detection of epileptogenicity	Deep learning
84	Raheja and Manoacha [96]	2020	To present an effective source for providing healthcare assistance with the help of global medical experts	Mobile telecardiology-based Method
85	Maji, Mandal [97]	2020	To develop an intelligent healthcare monitoring system	IoT, fiducial points and machine learning

3. Electrocardiogram

One of the most commonly used tools for clinical evaluation of the heart is ElectroCardioGram (ECG) due to its low-cost, simplicity, and risk-free operations [98, 99]. It

basically records the electrophysiological events in the heart, which is an indication of the electrical signal that are generated in the atria and ventricles through the process of depolarization and repolarization [99]. The P wave, the QRS complex, and the T wave are the three main components of the ECG signal representing one cardiac cycle during heartbeat [100]. Each wave form contains its interval and amplitude characterized by peaks and duration; this provides clinically useful information for cardiac arrhythmias detection [101, 102]. The analysis of these waves are also critically useful for the detection of commonly known breathing disorders like obstructive sleep apnea syndrome as well as for studying the autonomic regulatory process of the cardiovascular system during sleep and/or hypertension [103].

In computer-based ECG analysis, the accuracy of detecting QRS complexes is a necessary requirement. This task, however, is a difficult one due to interference with other internal noises such as muscular and motion artifacts, noises, and baseline drifts changes [104]. Differentiating other ECG component waves (i.e., P and T waves) from the QRS complex is another factor that increases the complexity of QRS detection [104]. Moreover, false detection of these component waves may cause incorrect results in computer-based ECG analysis. Several QRS detection algorithms have been developed by researchers in the last decades and have been applied in different application domains such as heart rate variability (HRV) analysis, arrhythmia classification, and heart rate estimation [105].

3.1. The ECG Waveform

The ECG is recorded as a reading of voltage versus time measured in millivolts (mV) and seconds. A representation of a traditional lead II ECG waveform is presented in Figure 3. It shows a sequence of peaks and waves that gives information about the depolarization and repolarization process of the ventricles or atria.

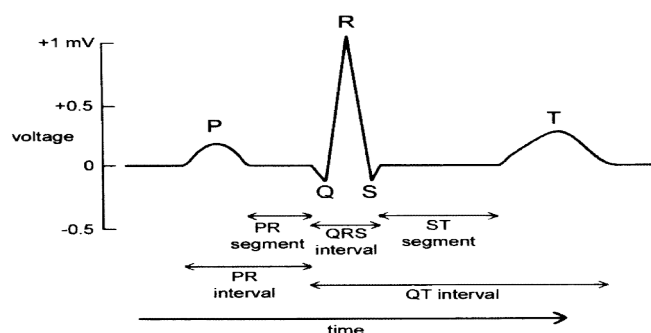


Figure 3. A typical ECG waveform for one cardiac cycle measured from the lead II position

The depolarization process of the cardiac cycle is initiated by the firing of the sinoatrial node in the right atrium of the heart. The atria then depolarizes causing the P wave to be produced. The P wave occurs in the interval of 80-100 ms duration. As the P wave terminates, this indicates the complete depolarization of the atria and following which there is contraction. The contraction then causes action potentials to spread across the atrioventricular node. Then, the left and right ventricles start to depolarize, leading to the production of the QRS complex. This represent the commencement of ventricular contraction and the end of atrial contraction. After the contraction the signal falls to baseline, the ventricles begin to repolarize after contraction, leading to the emergence of the T wave. This process is continuously repeated in the next cycle of the heartbeat.

Notable in the ECG waveform are several other regions which are of tremendous clinical importance. They include the P-R interval, the S-T segment, and the Q-T interval. The P-R interval is measured as the space in between the starting point of the P wave to the starting point of the QRS complex. The S-T segment is measured as the interval from the S wave component of QRS complex to the starting point of the T wave. The Q-T interval is measured from the starting point of the QRS complex to the end point of the T wave.

4. Expert System and Decision Support System

Decision Support System (DSS) is an information system that facilitates decision-making processes in a business or organizations, under specified conditions and constraints, to help humans decide on a particular issue (Rahamathunnisa & Chellappa, 2018). In recent years, several vendors under the trendy label of DSS have been providing a growing array of software packages to support management decision-making (Pfeifer & Lüthi, 1987). This significant development has been intensified using personal computers, developments in database management systems, and the introduction of “user-friendly” device interface techniques. Hasan, Ebrahim, Mahmood, and Ab Rahman (2017) classified DSS into five different types; Data driven, Model driven, Document driven, Communication driven and Knowledge driven.

Data Driven: This program focuses on the exposure and exploitation of large databases. The wide database includes history and organized data from both internal and external sources. Data-driven DSS helps decision-makers by analyzing large data volumes. Examples: computer-based databases which have to verify a query method (including data integration to add value to existing databases).

Model Driven: Every model-driven DSS build has a specific function as a different model is used for various sets of problems. Model powered DSS focuses on the access and manipulation of models. The main components of this kind of DSS are computational models such as representational models, accounting and financial models, and optimization models. Model-driven DSS does not need a big database. Instead, it only requires user-driven data and parameters.

Document driven: this type of DSS is more popular and it is targeted towards a large user group base. It is designed to search for web pages and find documents based on a user defined set of keywords or search terms to support the information need and use decisions of the user. The typical technology used for setting up the document-driven DSS is the client/server web architecture.

Communication driven: this is a type of DSS that improves user capabilities by promoting collaboration among people working on the same job. It is commonly used for other DSS forms.

Knowledge driven: Knowledge-driven DSS, through its problem-solving experience, offers help for decision-makers by recommending an effective solution to a problem. Artificial intelligence integration helps the problem-solving capabilities for this type of DSS. The framework uses a heuristic model (inference engine) to process the rules.

Decision support system presents some advantages to its users. Research has shown and substantiated a decreased decision cycle time, improved employee engagement, and more reliable decision-making knowledge for all types of decision support systems. The time savings reported by using computerized support for decision making are often significant. Another cogent advantage is enhanced effectiveness. Most studies have

analyzed soft measures such as perceived consistency of judgment, rather than quantitative measures. DSS also provides users with improved interpersonal communication; it can enhance coordination and cooperation between decision-makers. Communication-driven and group DSS have shown that effect in so many circumstances. Improved usability of data is also a significant impetus for developing a DSS powered by data. Worthy to note is the advantage of reduced expenses; some analysis and case studies have reported low cost for DSS from labour savings in decision making and reduced infrastructure costs. Moreover, in another perspective, learning occurs as a by-product of a DSS being used initially and continuously. Two forms of learning tend to occur: learning new ideas and gaining a deeper understanding of business facts for decision making. In fact, some DSS serve as de facto tools for training new employees.

In addition to the advancement of DSS, progress has also been made in the field of artificial intelligence (AI), where expert systems (ES) are being developed and, to some degree, used in decision making (Pfeifer & Lüthi, 1987). An expert system is a knowledge-driven application that usually models human knowledge to perform certain tasks in a particular problem domain. The systems process expert knowledge and seek to imitate their ideas, abilities, and intuitions. The definition of the expert system is generally based on the premise that the information of an expert can be stored in computer memory and implemented by a non-expert user. Tan et al. (2016), state that the distinctive characteristic of the expert system is an insightful capacity to analyze its logic and justify its decisions. Expert system is composed of several parts; Knowledge Base where the expert information resides; a domain-specific computer providing various types of inferences; an effective user interface; the query; and the advice generated by the system (Tan et al., 2016). The structure of an expert system is depicted in Figure 4, and each of its components are briefly introduced in the following subsection.

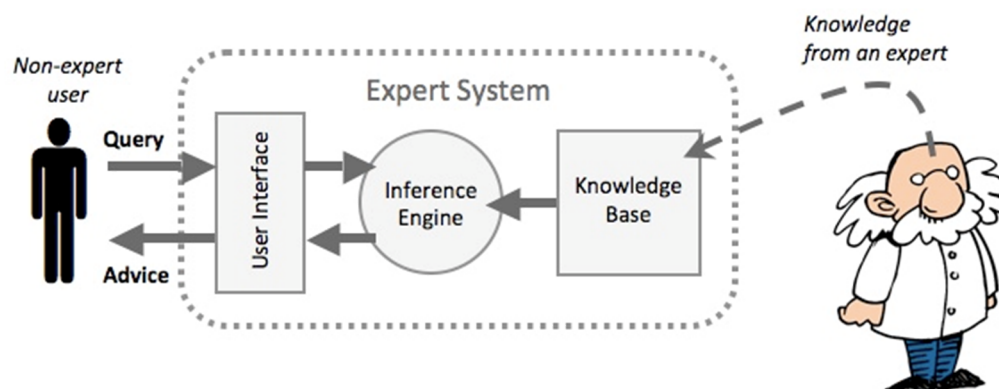


Figure 4. Components or Structure of an Expert system. Source [106].

Knowledge Base: the knowledge base is considered the core of the expert system; it comprises of rules and facts that model expert knowledge about the problem domain. It is a domain-specific information repository gathered from the human expert via the acquisition of knowledge. An expert system's knowledge base includes both empirical and heuristic knowledge. It replicates the expert's knowledge in the form of rules of development, frames logic, etc. [107].

Inference Engine: a significant element of any expert system is the inference engine. The inference engine is the component that determines how the expert system suitably interprets the information in the knowledge base. Its function is to work with the system and user data available to generate solutions to problems, extract knowledge, and produce answers, predictions, and recommendations from the database just as a human expert does. The inference engine works either in the forward or backward chaining

processes. In the backward chaining process, the system defines an expected solution, then tracks backwards to find supporting evidences for the selected solution. Thus, it is used when the solution is known. In the forward chaining process, the system collects data and works using a forward approach to find a suitable solution. It is often used when the desired outcome is unknown.

User Interface: The user interface component of the expert system controls the user-system interaction and communication. It provides facilities like menus, GUI, etc. that enables a nonexpert user to query the system and to receive feedback. Thus, it is an agent that enables the user to communicate with the expert system. The user interface function is to ease the use by developers, users, and administrators of an expert system.

Nagori and Trivedi [108] classify expert systems into five (5) different categories; Rule-Based Expert System, Frame-Based Expert System, Fuzzy Expert System, Neural Expert System and Neuro-Fuzzy Expert System.

Rule-Based Expert System: The rule-based expert system, as the name implies, consists of a collection of rules which is an expressive way of expressing knowledge. Expert knowledge is stored specifically as a set of rules in the expert system [108]. Through the years, a human expert can gather extensive knowledge and practical experience resulting in expertise. An expert can code the information as rules which are consequently used to develop the expert system. The rule consists of two parts: the antecedent represented by the PART(CONDITION) and the consequent represented as the PART (action). The basic syntax for the use of rules is as follows:

IF (antecedent)

THEN [Consequent]

Frame-Based Expert System: A frame is a structure of data that represents and models knowledge about a given entity or domain. In a frame-based expert framework, frames are used to capture and represent knowledge. Every frame has its name and an associated collection of attributes. The frame offers a natural means of expressing knowledge in a standardized and descriptive way that integrates all required information about a given object or concept. Unlike the rule-based expert method where systematic searching is done for all rules, in frame-based expert system, only frame scanning is done to execute rules.

Fuzzy Expert System: fuzzy set theory is commonly used to convey expert information that uses ambiguous and undefined terms. Fuzzy logic describes facts about entities on a sliding scale, which helps in distinguishing between class members and non-members. Fuzzy logic is also referred to as multivalued logic. Consequently, in fuzzy logic, all values of truth are represented through real numbers from 0 to 1. The probability that a given assertion is true or false is expressed by a number in the interval. The difference between the classical Boolean logic and the multi-valued fuzzy logic is depicted in Figure 5.

Range of logical values in Boolean and fuzzy logic

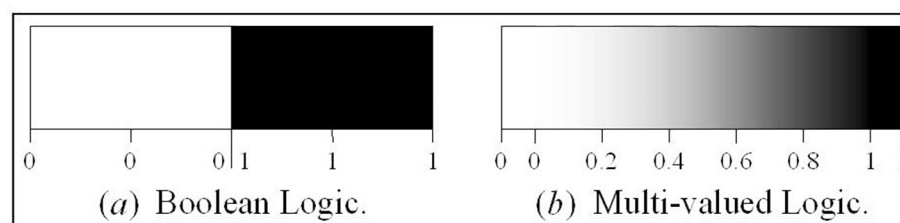


Figure 5. Fuzzy logic and Boolean logic

Neural Expert System: Instead of the conventional knowledge base, a neural expert system has a neural knowledge base, where information is stored as neuron weights. The combination of rule extraction based on a network of neurons (neural network) provides a learning facility for the neural expert system. The neural network also enables the handling of noisy and incomplete data due to its generalization capabilities. Thus, the expert system gives room for provisional reasoning. The rule extraction unit checks the base of neural information and generates rules that are implicitly embedded in the qualified neural network. The structure of a neural expert system is shown in Figure 6.

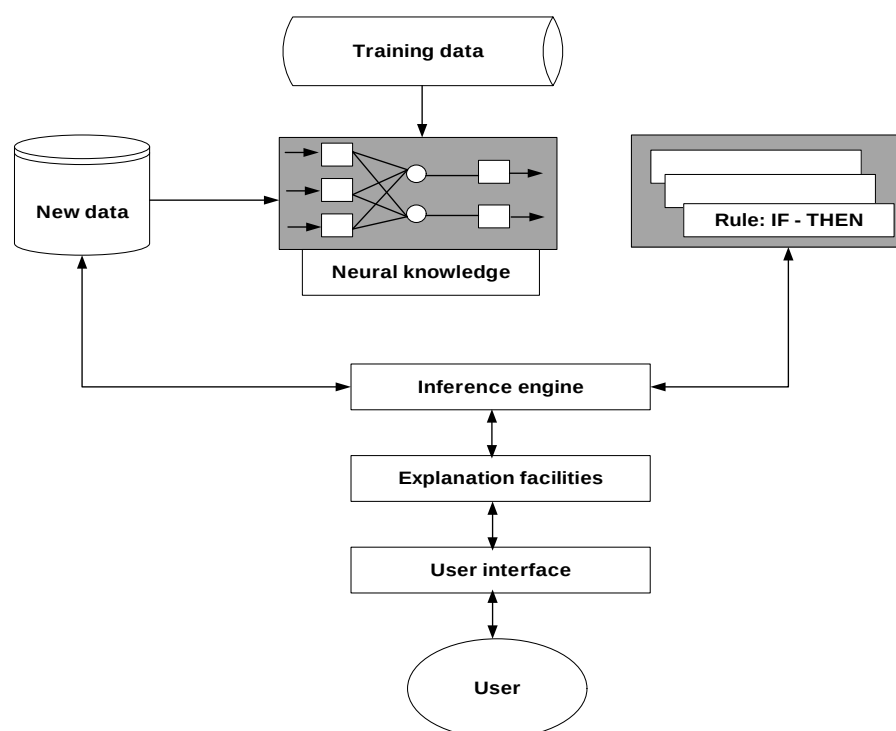


Figure 6. Basic structure of a neural expert system

Neuro-Fuzzy Expert System: Fuzzy logic and neural networks are complementary natural methods in the creation of intelligent systems. Fuzzy systems cannot learn and adapt to a new environment. While neural networks can learn, they use a black box mechanism which is opaque to the end users. However, when the neural network is combined with a fuzzy group of experts, it generates more efficient technologies for designing an expert group. Integrated neuro-fuzzy system combine neural network's parallel processing and reasoning with the human-like information representation and interpretation capabilities of fuzzy systems. The development of IF-THEN fuzzy rules

and the determination of membership functions for system input and output variables can be learned. Figure 7 presents the basic architecture of a neuro-fuzzy inference system.

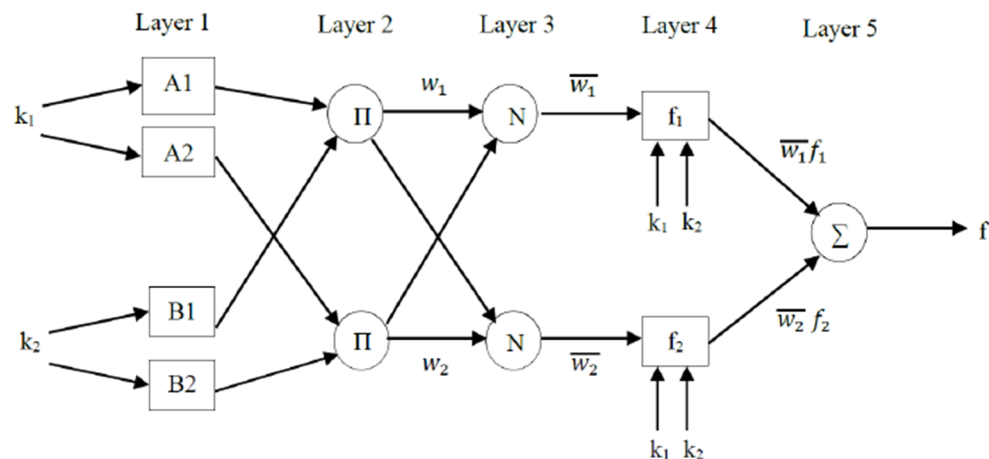


Figure 7. The architecture of a neuro-fuzzy inference system

4.1 Distinction between Decision Support System and Expert System

DSS and ES applications in domains requiring decision-making has increased significantly [19] but while DSS and ES are intended as strategies for enhancing decision-making, it is also true that there are strong and substantial variations between them. To recognize these variations, DSS and ES are compared in four primary areas: priorities and targets; organizational differences; users; and development methodology [19].

Priorities and Targets: DSS and ES essentially have the same fundamental goal; they aim to enhance decision efficiency. Nevertheless, their fundamental philosophies and priorities are quite different. The philosophy of DSS is to help the user decide by providing fast and easy access to appropriate data and models for that decision. ES, on the other hand, provides the user with a judgment that is always right. Since this is not feasible, an ES output standard is usually acceptable, similar to or better than the experts.

Organizational Differences: - DSS provides the user with the ability to modify data and templates in several ways when going through the decision-making process to solve an issue in a versatile way. With ES, relevant segments of the knowledge base are implemented based on the inference engine, control method durations, domain specific heuristics, and knowledge base data.

Users: Another major difference exists between the typical users. DSS is primarily implemented in a company or organizational environment. These are targeted at the efficacy of individuals in decision-making within a business organization. DSS is for a limited community of users. Expert systems, on the other hand, are generally concerned with science as opposed to business activities; users are predominantly scientists or scholars in a specific field of study.

Development Methodology: - DSS and ES are usually developed using a prototype or adaptive approach. Basic information and organizational specifications are defined when creating a working prototype. The selection of DSS approach is based on three

fundamental principles: a high degree of user participation, offering flexibility to the user's needs, and functional early-stage decision support. ES on the other hand, is developed through refinement and extension of the knowledge base to advance towards higher output levels.

5. Mobile Application for ECG Interpretation

Due to the advances in electronics technology and the development of digital signal processing techniques; many approaches have been introduced to design mobile applications for automatic recognition of heart abnormalities. Mobile application designs have majorly employed the use of photoplethysmography (PPG) and electrocardiograph (ECG) as the main concepts in measuring heart health and determining abnormalities [21]. ECG records the magnitude and direction of the electrical pulses generated by depolarization and repolarization of the heart vessels [99]. In-depth analysis of these electrophysiological events can be used to detect heart beat abnormalities and variations. The handheld ECG is composed of a mobile phone with a special mobile application interface to connect to an external ECG sensor unit. The ECG sensor is required for the mobile app to function effectively and adequately. On the other hand, PPG uses an optical technique that detects heartbeat by analyzing light absorption through changes in the skin color. Using a mobile app, the PPG sensor detects changes in light intensity via reflection from the body tissues (majorly finger and face tissues). This variation informs the happenings within the heart and can be used to detect abnormalities in the heart beat. There is also a reported dearth use of modern microelectromechanical (MEMS) sensors present in mobile phones based on an inertial measurement units for heart beat functional investigations [21].

5.1 Design Architecture of ECG Mobile Applications

Domazet, Gusev [26] presented generic design specification of a mobile ECG application as shown in Figure 8. The general architecture of the mobile application is composed of two actors (patient and doctor) and four ICT processing segments (acquisition, preprocessing/visualization, transmission, and interpretation/reporting).

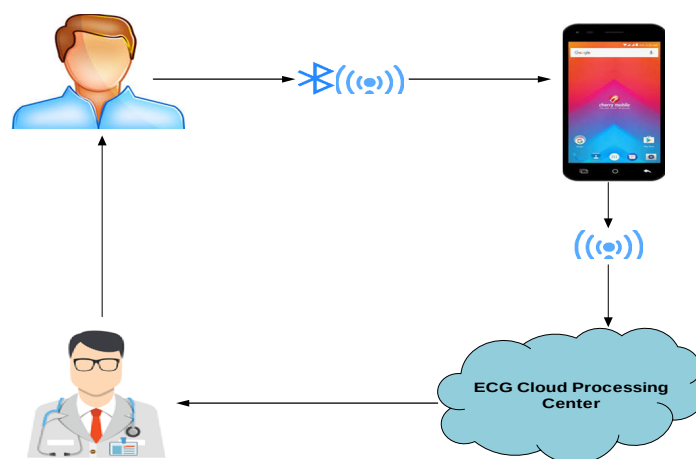


Figure 8. A Generic Design Architecture of ECG Mobile Application

The patient usually wears an ECG biosensor that collects real-time ECG data (acquisition). Mobile device is the second processing compartment for analyzing the collected ECG data. ECG data acquired by the biosensor is transferred to the patient's mobile device by employing personal area network communication, usually Bluetooth, Zigbee, or Wifi. The mobile device is responsible for reading the data and initial analysis

of the ECG signal. At this stage, visualization and monitoring of the patient ECG are carried out. After the initial preprocessing, the mobile device transmits the preprocessed ECG signal to the cloud for further sophisticated processing representing another segment. The transmission is usually done via a wireless broadband communication network. Further interpretation and processing such as presentation of detected QRS peaks, BPM rate, anomaly detection, and identification of extracted features and diagnosis are done in the cloud processing center by medical experts using sophisticated algorithms and techniques. Reports from this interpretation are sent back to the patient via the same channel.

Regarding the user interface of the ECG mobile applications, simplistic designs are employed due to public usage. The interface presents ECG visualization and a summary of apparent parameters for the visualization. Some applications carry out basic interpretation processes such as QRS detection, R-R interval detection, and heart rate measures on the mobile interface [20, 48, 109] so that users can have a quick grasp of their condition before transmission to cloud processing center for in-depth analysis or in the event of unavailability of cloud services. Most ECG mobile applications employ red-oriented colors for designing mock-ups or ECG traces to portray heart feeling [3, 24, 26]. Visualization is also implemented on the web application to be used by the cardiac patient and medical staff. A simple look of an ECG mobile application as extracted from Domazet, Gusev [26] is presented in Figure 9.

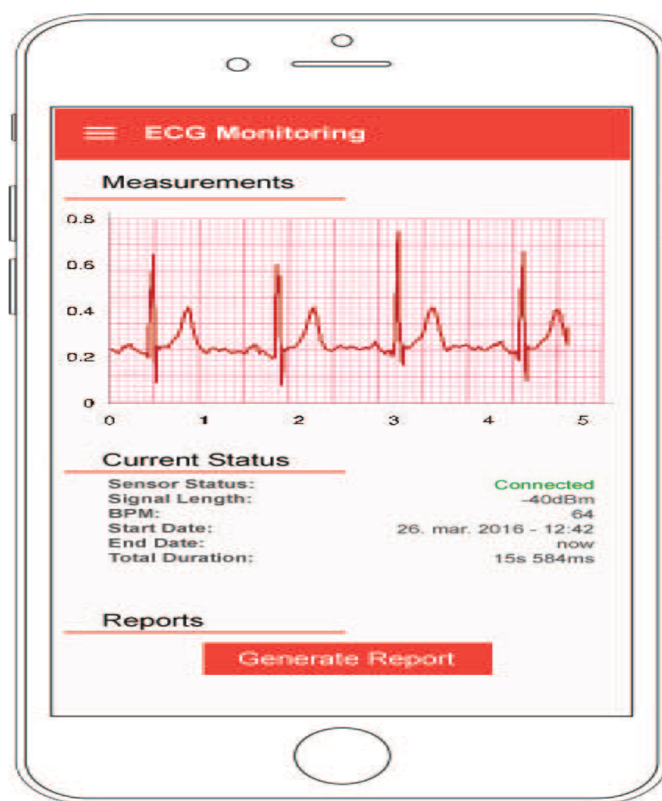


Figure 9. An example of ECG mobile Application Interface

Apart from presenting the ECG pattern of the patient, a mobile application interface is also used to present the report from in-depth analysis carried out at the cloud processing center to the user [43]. It is usually a summary of the analysis results that is sent as a report. Users receive the reports as an alert on the mobile application. Figure 10 shows an example of an analysis report alert on an ECG mobile application presented in [24].

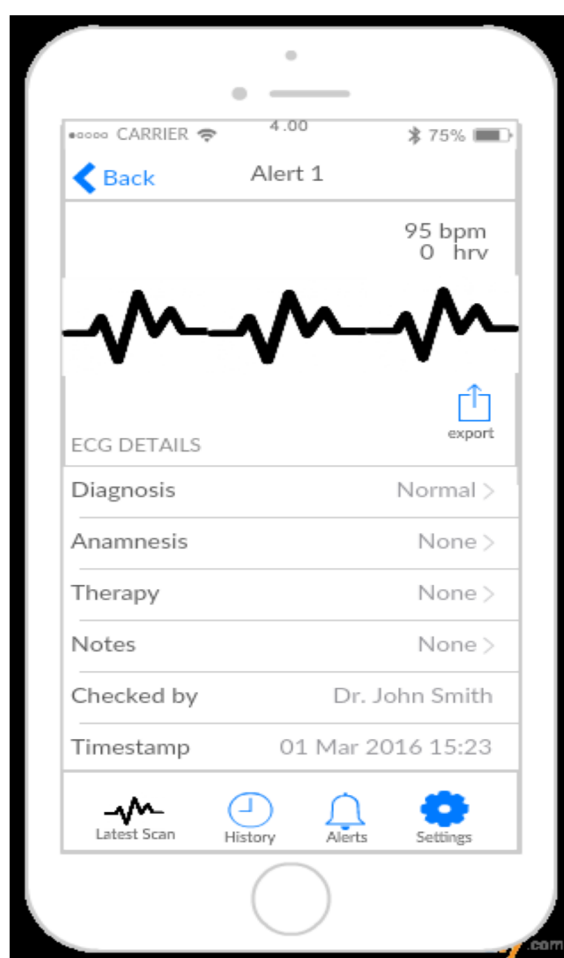


Figure 10. A Report Page on Mobile ECG Application

5.2 Appraisal of the Existing ECG Mobile Application

There is an upraise in the use of mobile smart phones since the beginning of the 21st century, and reports from surveys have revealed that over 100,000 mobile health apps and 400 wearable activity monitors exist on mobile stores (iTunes and Google Play) [21]. It was also reported that 62% of mobile phone owners in the United States use their phones to access health information about diseases and health conditions [21]. In recent years, there has been a notable upsurge in the number of mobile phone applications focusing on the management of cardiovascular diseases, some of which are based on measuring and analyzing ECG traces of patients. This section focuses on the appraisal of a representative sample of a selected mobile applications proposed in the literature and those available on the mobile stores for the acquisition and interpretation of ECG signals. This study identifies key features of mobile applications in the effective management and monitoring of heart disease patients via ECG interpretation. The features include: development platform, air interface connection, measured parameters, server upload capability, server type, market availability, and security of patient data. Table 2 presents the summary of the appraisal of the existing ECG mobile applications

Table 2 Mobile application for ECG Interpretation

Author	Title /App name	Objective	Development Platform	Data Acquisition interface	Measured Parameters	Heart disorder detected	Uploaded capability	Server type	Market availability	Patient data security
AliveCore Inc	kardiaMobile	Captures a medical-grade single lead ECG signal to detect heart rhythm	Android and iOS	Ultrasound	ECG traces, Heart rate	Atrial Fibrillation, bradycardia, tachycardia	Yes	E-mail	Paid	Yes (with premium subscription)
AliveCore Inc	kardiaMobile6L	Captures a medical-grade 6 lead ECG signal for comprehensive analysis heart condition	Android and iOS	Ultrasound	Detailed ECG traces, Heart rate, weight, blood pressure	Atrial Fibrillation, bradycardia, tachycardia	Yes	E-mail	Paid	Yes(with premium Subscription
IMED Kft (2013)	Cardiax Mobile ECG	A companion application designed for cardiac health monitoring with 12 channels / Lead	Windows and Android	Wifi	ECG traces, Heart rate, QRS complex, Pd, PQ	Sinus Rhythm, Arrhythmias	Yes	Email and FTP server	Open	None
Ardas (2015)	cardiolyse	A healthcare mobile application	Java and Android	OTG USB cord	ECG tracs and other 17	None	Yes	SaaS server	Paid	None

		n to connect with existing cardio appliance device			parameters					
VitalSignum Oy (2019)	Beat2Phone	Mobile application for 1 lead ECG signals to monitor heart rate and posture A 12-Lead Mobile application for interpreting ECG signals develop a prototype android	Android	Bluetooth	ECG traces, Heart rate, HRV. Gps location Timestamp		Yes	FTP server	Paid	None
Cardioline S.p.a (2017)	TouchECG	application for interpreting ECG signals develop a prototype android	Android	Bluetooth	ECG traces, heart rate	Arithmias	Yes	E-mail	Open	Yes
(Prerana, Cheeran, & Sharma, 2014)	Android application for ambulant ECG Monitoring	ECG application compatible with the available ECG acquisition device	Android	Bluetooth	ECG traces, QRS complex, Heart rate	None	Yes	FTP Server	Unknown	None
(Brucal, Clamor, Pasiliao, Soriano, & Varilla, 2016)	Portable Electrocardiogram Device Using Android	To analyze and interpret ECG signal from	Android	Audio Jack	ECG in .3gp format, BPM, heart Rate, R-R interval	None	Yes	Unknown	Unknown	None

	Smartph one	portable device using android smart phone									
(Stojmen ski et al., 2016)	A mobile applicati on for ECG detectio n and feature extractio n	develop a proof-of-c oncept system for heart attack detection using ECG sensor. Propose a remote monitorin g system of electrocar diogram and heart rate using Android smartpho ne. The	Androi d	Bluetooth	ECG traces, BPM, HRV GPS Location Timesta mp	Heart attack, anamnesis	Yes	FTP Serve r	unknown	None	
(Utomo & Nuryani , 2017)	QRS peak detectio n for heart rate monitori ng on Android smartph	Develop a smart mobile ECG system for monitorin g the heart health of elderly people	Androi d	Bluetooth	ECG trace, QRS Complex, heart rate	None	No	None	Unknown	None	
(Teja & Rao, 2018)	A Smart Wearabl e System for ECG and Health Monitori ng	MIT APP Invento r for Androi d		Bluetooth	Temperat ure, Heart rhythm, Heartbea t, Blood Pressure, GPS Location Timesta mp	None	No	None	Yes	None	

It can be observed that the majority of the mobile applications use Bluetooth as a connection medium for raw ECG signal acquisition except ALiveCore's CardiaMobile, IMED Kft's Cardiax and Ardas' Cardiolysse that uses Ultrasound, Wifi and OTG USB connectors as the acquisition medium. Similarly, most of the apps are android-based with the exception of CardiaMobile, that is, cross platform and Cardiax for Windows and Android. Due to the computational capability of mobile smartphones, mobile application for ECG measure a limited number of parameters of ECG traces, heart rate and QRS cutting across all identified apps both on app stores and published literatures. Some Mobile Apps, especially the ones presented in published journals, measure some other patient non-ECG parameters that could aid heart disease diagnosis such as temperature [110], BPM [20, 24] and blood pressure [110]. It is also observed that some of the mobile apps include GPS location timestamps in the captured data so that remotely monitored patients can be timely rescued in emergency situation [24, 110].

It is also noticed that few of the mobile apps are used to detect heart rate abnormalities directly. Majority of them only preprocess the ECG signals and send to the cloud for in-depth analysis to detect heart beat abnormalities. This might be due to the complex property of ECG signal which requires sophisticated algorithms that mobile devices cannot handle. Nevertheless, CardiaMobile, Cardiax, and TouchECG possess the functionality to detect certain heart beat abnormalities such as limited types of arrhythmia, sinus rhythm, and heart attack. In terms of the security of the patient data, the majority of the mobile apps available did not provide any encryption techniques for protecting sensitive health-related data of users from unsolicited and unverified access. The few that provide this security functionality requires a premium subscriptions which many users may not be able to afford.

6. Taxonomy of features for ECG interpretation and diagnosis

Cardiovascular diseases and their diagnosis from ECG offer significant advancement in medical domains. ECG has been widely utilized in the diagnosis of numerous cardiac abnormalities. A cardiac cycle in an ECG signal corresponds to the P–Q–R–S–T waves as discussed in Section 3. This cycle can be compactly termed as P, QRS complex, and T waves [74]. The electrical activity of the heart, as represented by the cardiac cycle of the ECG waveform gives the individual heart beat which even the patient can perceive. This is made of various electrical depolarization-repolarization process [18]. This signal pattern can be explored to detect a variety of diseases such as CVD. Deviation in ECG signal parameters from their normal values is usually caused by cardiac abnormalities. Therefore, experimentally, this point is exploited by researchers through the analysis of ECG signals to detect and diagnose CVD and identify patients suffering from the disease without any surgical intervention. This approach has been shown to reduce human interpretation of ECG tracings and increase detection accuracy [18, 32, 55].

ECG signal has been characterized with different types of noise, which hinders the extraction of discriminative ECG features or characteristics to develop ES and DSS system for heart disease diagnosis. In addition, the temporal variations of physiological conditions also contributed a lot of factors towards developing an effective algorithm for ECG feature extraction [37, 55]. Thus, ECG signals must first be subjected to the preprocessing phase before the features of interest can be extracted for analysis.

6.1 Noise and Noise Cancellation Techniques for ECG signals

There are basically two main classes of noise that affect ECG signals. These include low frequency baseline wander and high frequency random noises [30]. The former is caused by the movement of the respiratory tract and body movements. The latter, high frequency random noises are caused by mains interference, which is 50 or 60 Hz [111]. In addition, the causes can also includes muscular activity, motion artifacts, random shifts of the ECG signal amplitude usually created as a result of poor electrode contact and body movements, and other interruptions of the original recorded ECG signal [18, 30, 79]. Figure 11 shows a sample ECG signal with and without noise. To eliminate low frequency baseline wander, linear filtering and polynomial fitting (cubic spline filtering) techniques have been used [30]. In linear filtering, time-invariant high-pass filter is developed and a cutoff point is chosen to preserve clinical details in the ECG as well as guarantee the removal of baseline wander. The lowest heart rate at around 40 bpm is chosen during bradycardia, which specifies around 0.67Hz - the lowest frequency component in the ECG signal. The cutoff frequency can then be set at around 0.5Hz. Low-pass filter has been widely used to suppress power line interference [79]. Jung and Lee [73] proposed Daubechies 4 (db4) wavelet to extract baseline wander and noise from the original ECG signals. Hejazi, Al-Haddad [74] proposed Discrete Wavelet Transform (DWT) of Coif3 family with Rigrsure rule of hard thresholding technique to denoise ECG signals. Pass-band filter with frequency values between 0.67 Hz and 45 Hz has been used to remove respiration and power line noise in the ECG signals [32].

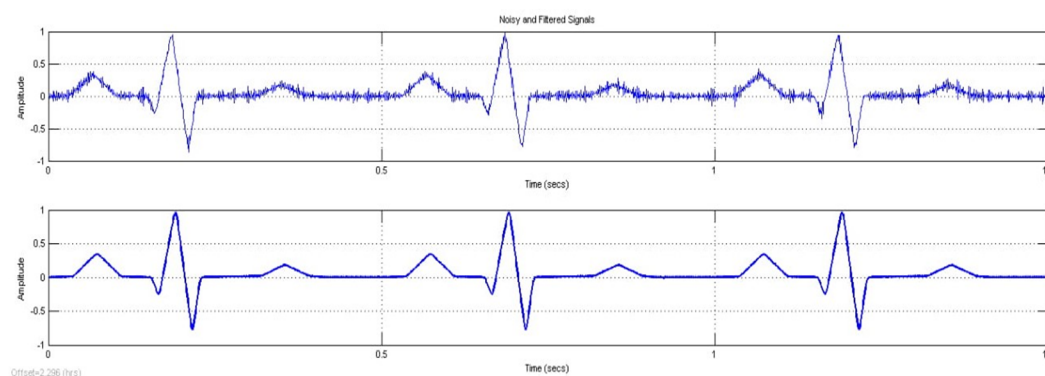


Figure 11. ECG recording with and without noise (Source: Bellos, Papadopoulos [30])

Conversely, polynomial fitting, also referred to as cubic spline filtering, involves the fitting of polynomials to representative points (knots) on the ECG, where one knot is used for each beat. These knots are chosen from a “silent” segment, such as the PQ interval. This fitted polynomial passes through each knot in a smooth fashion [30, 85].

In biomedical and telemedicine domains, the wireless transmission of ECG signals is mostly affected by noise owing to improper channel. This noise is modeled as white Gaussian noise, which can be regarded as a conventional frequency noise. The noise is added to the pure ECG signals and requires a filtering technique for effective removal. A number of filtering techniques for white Gaussian noise have been studied. These include the application of Wiener and adaptive filtering techniques [112]. Wiener filter is an optimal filter that is mostly useful when the power spectrums of the input signal and noise overlap and cannot be separated by the traditional low-pass filters. Despite Wiener optimal performance, its computational complexity remains a major challenge [113]. Adaptive filter was introduced to provide better performance over Wiener filter. Different types of adaptive filtering techniques like Wavelet, Empirical Mode Decomposition (EMD) and Recursive Least Squares (RLS) have been explored to remove noise in ECG signals [58]. Stochastic gradient Mean Square (LMS)-based adaptive filtering has been used for white Gaussian noise removal to reduce energy consumption

in signal processing [85]. However, LMS-based adaptive filtering requires a large step size to produce good filtering performance. One of the major setbacks of the adaptive LMS algorithm is the fixed step size parameter requirement for every iteration, which greatly affects the filtering performance [18, 112]. To improve the performance of the filtering process, an LMS algorithm with normalized step size is proposed in a number of studies [18]. Venkatesan, Karthigaikumar [18] introduced a delayed error normalized LMS (DENLMS) adaptive filter algorithm for ECG noise cancelation with moderate computational complexity. DWT has been used in research work of [67] to denoise ECG signals. Preprocessing of ECG signals has attracted research attention in various bioinformatics applications. After preprocessing, the next phase is feature extraction from ECG signals.

6.2 Feature extraction from ECG signals

The performance of medical ES and DSS relies entirely on the quality of the features used to develop the knowledge-base [34, 82]. As such, care must be taken when extracting features from ECG signals. Figure 12 shows the taxonomy of the different features that have been used to develop ES and DSS systems for ECG interpretation and diagnosis. These features can be broadly classified into three: fiducial, non-fiducial, and hybrid feature extraction approaches. The subsequent section provides detailed information on each feature category.

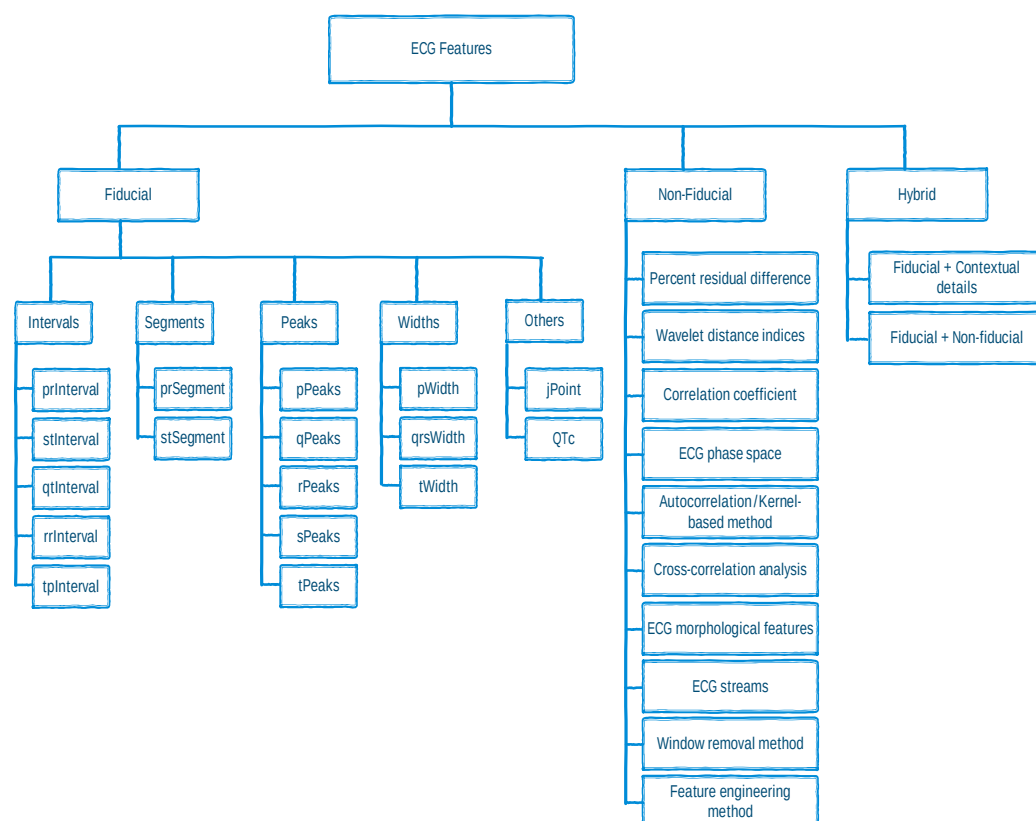


Figure 12. Taxonomy of features for ECG interpretation and diagnosis

6.2.1 Fiducial Features Extraction Approaches

Fiducial feature extraction approach extract features from the physiological signals. Fiducial-based approaches are techniques used to extract the characteristic points of the ECG signals in time-domain [55]. ECG normal signal contains specific waves, consisting of P, QRS complex, and T waves. Heart atria depolarization is depicted by P wave; a positive, low-frequency and low amplitude signal. Conversely, ventricle depolarization is depicted by the highest amplitude and the highest frequency of ECG waves as described by the QRS complex. At the end of the cardiac cycle, the T wave is used to depict the ventricle repolarization. These waves form the basis for the distinctive points of the ECG-recorded signal, which are P, Q, R, S, and T. To extract the salient fiducial features for effective ECG interpretation and diagnosis, the onset, offset, amplitude, duration and gradient of each wave are explored [6]. When dealing with fiducial feature extraction, the algorithm used for extracting the salient characteristics of ECG signals must determine the precise boundaries of the waveforms. Based on the suitable combination of P, Q, R, S, T waves, several features of ECG can be determined. For instance, Mahmoodabadi, Ahmadian [37] extracted six fiducial-based features from ECG basic waves (i.e, P, Q, R, S, and T). The extracted features: P–R, QRS, R–R time intervals, heart rate, R–R time interval variation, and T–P and S–T interval voltage levels, were used to train a fuzzy classifier implementing Takagi-Sugeno-Kang (TSK) fuzzy inference system based on 48 ECG signal records. The proposed classifier was used to detect 14 classes of arrhythmia [37]. ECG signal features consisting of P, Q, R, S, T waves and the zero level of the signal are extracted first with the use of wavelet transform.

To extract the fiducial features from ECG waveforms, R-peak (QRS complex) detection is very crucial. The detection of R-peak will help in the calculation of two important feature parameters. These parameters are Interbeat (RR) interval and the Heart Rate Variability (HRV). The abnormality of heart rate or its variations, which exists in the morphological pattern, is a sign of an arrhythmia. This variation in the morphological pattern can be detected through the analysis of recorded ECG waveforms. HRV is the most powerful and useful feature extracted from ECG signal variations for detecting cardiac disorders and associated diseases [18]. The most widely used R-peak detection algorithm in the literature is Pan-Tompkins algorithm [30, 58, 79]. This algorithm involves analysis of the slope, amplitude and width of QRS complexes in the ECG signals. It includes several filtering techniques that accomplish high-pass, low-pass, squaring, derivative, integration, search operations, and adaptive thresholding. Lee, Jeong [79] proposed polygonal approximation method to extract fiducial features. Manriquez's method for fiducial feature extraction is based on a threshold value of the auxiliary signal produced from Hilbert transform. The popularity of DWT has made it useful in the analysis of ECG signals.

DWT based R-peak detection technique has been employed specifically for the reduction of the computational complexity in the feature extraction phase of ECG interpretation [18]. Several wavelet transforms have also been used for the detection of R-peaks in ECG signals. However, in most of the feature extraction processes, selecting the mother wavelet is very vital to improve performance. For instance, Venkatesan, Karthigaikumar [18] selected Coiflet wavelet to detect QRS complexes in ECG signals. Coiflets are wavelets formed from Daubechies wavelet family, which has a closed resemblance to QRS complexes and possesses low frequency energy spectra [37]. Coiflets are more symmetric in nature with a near linear phase and are characteristically better than Daubechies wavelet and Spline wavelet [18]. Israel, Irvine [114] extracted 15 fiducial points from ECG signal after detecting P, QRS complex, and T waves. The authors applied Linear Discriminant Analysis (LDA) to classify 29 subjects. The results show that 100% subject recognition is possible using the extracted fiducial features. 82% ECG beat recognition rate was achieved using this approach [73]. Thirty (30) fiducial point features have been proposed in the work of Biel, Pettersson [115]. The authors

applied Soft Independent Modeling of a Class Analogy (SIMCA) classifier for comparison of unlabeled samples with the data pertaining to a trained group. This method was proposed for classification of a subject with the appropriate well-matched class label. The experiment was carried out using a total of 20 subjects and a recognition rate of 100% was achieved [73].

In most of the existing rule-based ES for ECG interpretation, clinicians are not able to externally access the rules used by these systems. As a result, the ES and DSS become black-box. In order to solve this problem, Bond, Finlay [31] proposed a number of fiducial-based features by studying intervals, segments, peaks, widths, and some features based on heart rate and the cardiac axis to build a rule-based eXtensible Markup Language (XML) framework for ES, which can be used for interpretation of ECG signals. The rules mined from ecgRuleML proposed in this study can be accessed externally by clinicians to have an understanding of the underlying decision rules used by the ES when diagnosing patients with heart-related diseases. An ecgRuleML document represents a readable (both to human and machine) rule-based expert knowledge. DCT and DWT have been applied in the work of [58, 67] to process R-peak data extracted using Pan-Tompkins R-peak detection algorithm. By analyzing ECG signals obtained from MIT-BIH arrhythmia database, Daubechies (db4) mother wavelet based multiresolution analysis has been applied to decompose the signal into nine stages of subbands. The ninth stage approximation coefficient of the frequency band between 0 and 0.351 Hz refers to the baseline drift. Because the ECG signal does not have any important data above 45 Hz, the initial two levels of the wavelet coefficients are set to 0. The remaining wavelet coefficients in the detailed subbands (third to ninth level) are reconstructed to get the resultant filtered ECG. The R-peak extracted data are divided in such a way that the individual division contains 99 and 100 samples before and after the R-peak, respectively. ECG beats of 200 samples, which belong to five categories of arrhythmias have been utilized by the authors [58].

Moreover, a certain numbers of abnormal features are difficult to represent numerically and as such the characteristic element can be used instead to depict abstract features like M shaped P waves and slurred S waves and [32]. While the use of fiducial features has helped in studying the various significant points in the ECG signals, this approach requires precise detection of boundaries. Obtaining effective boundaries has been really challenging due to the variations in ECG signals and the presence of different types of noise. In addition, this approach has been reported to be computationally challenging [32]. As such, the use of non-fiducial feature extraction approaches has been extensively studied.

6.2.2 Non-fiducial Features Extraction Approaches

Unlike the time-domain analysis used in the fiducial approaches, non-fiducial feature extraction techniques obtain features from a transformed domain using Fourier or wavelet analysis. Non-fiducial approach was introduced to resolve the shortcoming of the fiducial point-based feature extraction approach. As we oppose fiducial point-based approaches, non-fiducial methods do not require determination of the precise boundaries of the waveforms. This approach extracts differential data within ECG waveforms with no conspicuous fiducial points [32, 73]. Although, studies have shown that both fiducial and non-fiducial approaches exhibit similar results in terms of performance based on a comprehensive performance evaluation study conducted by Odinaka, Lai [116]. However, more research effort is needed to validate this empirical finding. In essence, non-fiducial approaches employ a windowing method where ECG signal in time-domain is decomposed into windows using the time interval as the possible minimal manipulation that can be performed on the signal. Each segmented window is then

subjected to a transformation to extract a number of coefficients, which will lead to the feature of interest. These features can be used to detect the rate of heartbeat. A typical example of window segmentation for non-fiducial approaches is shown in Figure 13. In this figure, ECG signal is partitioned into segments and each segment is studied separately. Majority votes of the detection result obtained from each window can be used to categorize the patient [73]. In the data stream environment, the transformed windows can be subjected to buffer and unbuffered approaches as shown in Figure 13.

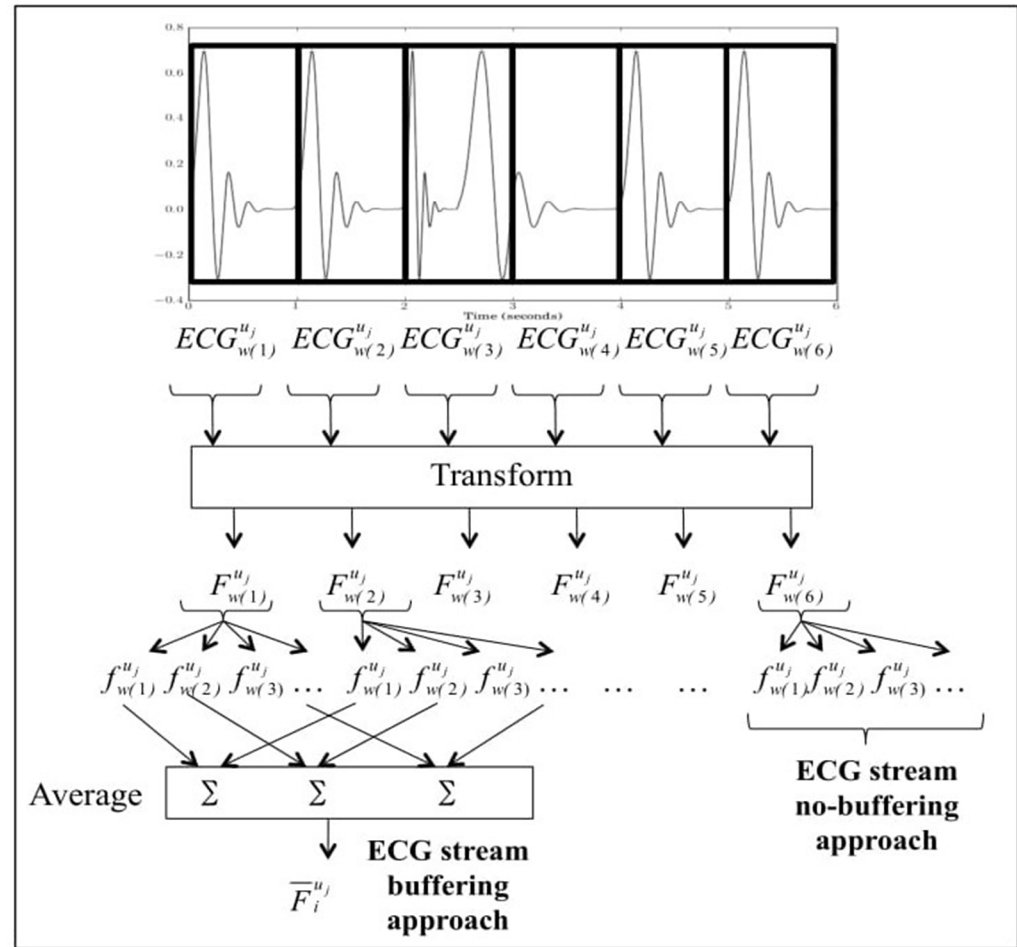


Figure 13. Windowing method and ECG streams proposed in [32]

Camara, Peris-Lopez [32] proposed ECG stream method to extract non-fiducial features from ECG signals. They proposed a continuous authentication ES by considering ECG signals as continuous data streams. The dataset for the experiment is based on 10 individual records selected from MIT-BIH Normal Sinus Rhythm database. K-NN algorithm, with $K = 1$, was used to perform the final classification of the patient's health status. In their study, Walsh-Hadamard transform is then utilized to transform the resultant windows. This transformation performs a projection of a signal onto a set of square waves, which is referred to as Walsh function. Performance accuracy of 96% was reported from the experimental investigation. Despite the impressive results, the proposed algorithm cannot be generalized as the system's performance was only evaluated on 10 records of individuals. The performance of different non-fiducial approaches such as percent residual difference, correlation coefficient, wavelet distance indices, ECG phase space, kernel-based method, cross-correlation analysis, and ECG

morphological features has been reported in the literature [6, 73]. For instance, the performance of three non-fiducial approaches has been explored in the work of [117]. These approaches include distance measurement using wavelet coefficients, correlation coefficient, and percent residual difference. The experiment was conducted on 50 subjects and an accuracy of 89% has been achieved. The authors reported that the approach based on distance measurement using wavelet coefficients outperformed the other two approaches. However, despite the remarkable success achieved in this study, the detection accuracy still needs further improvement and the proposed approach has been characterized to be highly sensitive to ECG segment length [6].

Distance measurement using wavelets has also been studied in the work of [117] and [118] as reported in [73]. Chan, Hamdy [117] proposed a framework that is based on non-fiducial feature extraction approach with the aid of wavelet transform distance. The study analyzed 50 subjects and reported an accuracy of 89%. Chiu, Chuang [118] proposed an individual identification technique with 512-point feature extraction using Euclidean classifier and wavelet transform. Recognition rate of 100% was reported on 35 subjects belonging to the normal class and 81% recognition rate for 10 subjects belonging to the arrhythmia class. Similarity as well as dissimilarity measures between ECG phase space portraits has been studied for the development of human identification ES. The system achieved an accuracy of 99% using a three-lead ECG configuration. However, it was reported that when the number of leads was reduced to one, the accuracy of the system dropped significantly to 93% [6]. A tunable Q-factor wavelet transform (TQWT) and spectral feature analysis has been proposed in [64] to build a DSS for automatic sleep staging based on Electroencephalography (EEG) signals. The authors split EEG signals into wavelet subbands using a tunable output factor and spectral characteristics derived. The study applied wavelet transform for extraction of features and used a random forest technique for the grading stage. The authors used time-frequency features to extract specific spectral features from subbands of the TQWT. The experiment was conducted on 28 subjects and an accuracy of 90.38% to 97.50% was reported for 6-class and 2-class, respectively.

In the field of identity recognition using ECG as a physiological trait for security, ABC proposed an autocorrelation and kernel-based approaches for feature extraction and dimensionality reduction of ECG signals. The features extracted using this approach were used to train a one-class Support Vector Machine (SVM) to learn the individual pattern in the ECG signals. Autocorrelation method is applied on an individual nonoverlapping windows to detect discriminative feature vectors. The ECG data have been windowed into 1028 coefficients at 5 sec duration. For reducing the dimensionality of these feature vectors, a different dimensionality reduction method was evaluated, which includes kernel-based PCA, Principal Component Analysis (PCA), and Linear Discriminant Analysis (LDA). The reduced features were from the one-class SVM for subject classification. The authors reported that Kernel-based PCA produces the lowest error when tested on both binary and one-class SVM.

It has been reported that during the windowing section of non-fiducial feature extraction approach, unnecessary signals may be present other than those normal ECG signal, leading to a reduction in the overall recognition rate. This may also affect the individual window identification rate. The presence of these distorted signals can be solved by analyzing all windows generated and remove, those windows that may be difficult to recognize or those windows that have unwanted signals. To address this issue, Jung and Lee [73] proposed window removal approach, which applied DCT to all generated windows. Threshold value is used to filter windows that do not certify the condition. After removing the unnecessary windows, the extracted non-fiducial features were used to train three classification algorithms (Nearest Neighbor, SVM, and LDA).

Experiment was conducted using Normal Sinus Rhythm, PTB Diagnostic, and QT databases. This research shows that the recognition rate of both subject and window can be improved by removing unnecessary windows and signals from the decomposed ECG signals.

6.2.3 Hybrid Features Extraction Approaches

ECG interpretation and diagnosis in medical applications have been shown to be very difficult due to the underlying characteristics of ECG signals. As such, a single feature extraction technique may not be sufficient when analyzing all manner of ECG data. Consequently, researchers have explored the possibility of performing hybrid feature extraction to improve the resultant classification performance of the recognition algorithms. To develop a robust ES and DSS, ECG signal analysis requires appropriate features and classifiers to categorize patient health status. For instance, Alshraideh, Ootom [55] has combined ECG characteristic points with patient's demographic data as input to a web-based DSS to detect a patient suffering from heart problems. Cardiac arrhythmia data obtained from the University of California was used to evaluate the system. A dataset of 279 attributes and 452 instances which are spread among 16 types of arrhythmia classes was developed. Five classifiers have been used to classify the different classes of arrhythmias considered in this study. These include J48 decision tree algorithm, Jrip rule-based algorithm, Kstar nearest neighbor algorithm, SVM, and Artificial Neural Network (ANN). The authors applied Synthetic Minority Over-sampling TEchnique (SMOTE) filter in WEKA to produce duplicates of the minority classes. J48 algorithm has shown the highest classification accuracy of 98.29%.

Venkatesan, Karthigaikumar [18] has explored the possibility of combining fiducial features with non-fiducial by extracting 14 time-domain and frequency-domain HRV features from ECG signals. In essence, three important frequency regions are present in the human HRV signal. These include high frequency (HF), low frequency (LF), and very low frequency (VLF). VLF is below 0.04 Hz. LF varies between 0.04 and 0.15 Hz and HF is from 0.15 to 0.5 Hz. Six frequency-domain features were added to the eight time-domain features to identify abnormal heart rhythm. The frequency-domain features, which were extracted using NI LabVIEW biomedical kit include LF Power, HF Power, VLF Power, HF norm, LF norm and ratio of LF to HF. Experimental results based on SVM classification algorithm yielded a maximum accuracy of 96% for classifying normal and abnormal subjects based on the ECG dataset collected from MIT-BIH database. Bellos, Papadopoulos [30] has combined frequency-domain features such as LF, HF, and the ratio of LF to HF along with features collected from various wearable sensors to develop a rule-based DSS for heart disease diagnosis. The authors developed a system that collects and analyzes information applicable for predicting the severity of a health condition of patients suffering from chronic diseases using wearable sensors. The system used multiparametric sensor data which include ECG, motion, oxygen saturation (SpO₂), respiration, temperature, among others. A smart assistant device was integrated which is responsible for analyzing the collected multiparametric data and simplifying the monitoring of patients. After preprocessing, the smart assistant device integrates all collected data from sensors with the patient's information. The authors evaluated the feature extraction stage using two recordings with each less than 2 hours. These samples were taken from 2 subjects and their annotation was performed by a physician. Three R-peak detection methods were tested and evaluation metrics such as correctly identified R peak, false positive R peak, false negative R peak, and absolute percentage error were used. These features were applied to develop the rule-based DSS. In the classification

phase, 10 fold cross-validation method was used for testing based on different classification algorithms like PART J48, Random Tree, and Naive Bayes.

Minutolo, Sannino [28] also presents a rule-based DSS for mHealth environments specifically for cardiac heart monitoring. The system detects and signals abnormal or emergency situations by using hybrid features based on contextual information such as the patient's posture and physical activity and data from a wearable ECG device. The rule-based DSS encodes high-level and specialized knowledge gathered from clinical experts for cardiac diagnosis and monitoring. The DSS makes inferences from a simple mobile reasoner with the goal of detecting potentially dangerous situations. The features used by the system belong to five main categories: patient summary, heart monitoring information, physical activity information, posture information, and alert information. Ontology was introduced to represent this information. The overall architecture of the proposed system is segmented into three different layers, namely; Data Layer, Decisional Layer, and Action Layer. Data layer is responsible for collecting sensor data and representing them in the form of ontology description. The Decision layer is responsible for using the expert knowledge formalized in the ontology and production rules to recognize the possible critical situations and determine the suitable actions to be carried out by the Action Layer. Action layer executes the actions inferred by the Decision layer through the implementation of mechanisms to generate reactions like alarms and feedback messages. To verify the system performance, the authors conducted a number of tests using a set of hardware devices. These include an all-in-one wireless ECG and activity monitor (i.e, Alive Heart Monitor device), a smart phone, and a patient simulator (i.e, Datrend Advanced Modular Patient Simulator (AMPS-1)). They examined a set of 15 healthy people consisting of 80% men and 20% women with ages from 25 to 48years.

Khatibi and Rabinezhadsadatmahaleh [87] proposed feature engineering method to extract hybrid features from ECG signals. In this study, four classes of arrhythmias were detected using a feature engineering technique that utilizes deep learning, fiducial points and K-NN. The features learned from pretrained deep learning Convolutional Neural Network (CNN) architecture were used alongside handcrafted fiducial point-based features and K-NN features from the feature engineering approach. SVMs with different kernels and decision trees were employed to classify the features extracted by the proposed method. The model showcased very competitive performance result for beat classification and achieved an average accuracy of 99.77%, AUC of 99.99%, precision of 99.75%, and recall of 99.30%. The strength and suitability of the proposed method is revealed in the high balance between sensitivity and specificity. The experiment was conducted using MIT-BIH dataset of 48 recordings from 47 patients. They used the annotation file for segmenting the ECG signal to its beats.

The justification for using wavelets Fourier transform in the biomedical domain has been critically studied. Fourier transform analysis generates ECG signal spectra or a range of frequency amplitudes that exist within the signal and can only provide the spectral components of the signal without considering their temporal relationships. Conversely, wavelet signal analysis can produce a time versus frequency representation of the ECG signal, and this approach has been considered effective when dealing with nonstationary data. The availability of many wavelet functions enables a robust search space for wavelets that will successfully represent a signal of interest. It has been reported that the algorithms employed for implementing DWT are even faster than the fast Fourier transform under the same conditions [37].

7. Taxonomy of methods for ES development in ECG interpretation

Nowadays, ES has become a new shift in biomedical and bioinformatics technology. This is due to the fact that ES achieves good performance in a specialized problem domain (such as medical diagnosis) that is considered difficult and requires specialized expertise and skills. It does so by processing the knowledge of medical experts and trying to mimic their skills and intuition. Recently, ECG interpretation has witnessed increase in the application of ES in developing decision support systems for diagnosing and monitoring patients with heart diseases [5, 63, 71, 119-122]. Different methods and approaches have been applied to the modelling, design, and development of ES-based decision support systems in ECG interpretation for the diagnosis of heart diseases. This section focuses on the taxonomy and review of ES methods and developmental approaches in existing literatures for ECG interpretation.

In Figure 14, the identified taxonomies along with the different methods employed under each taxonomy and their frequencies for the past decade are presented after a thorough review of the existing works. Seven ~~(7)~~ different approaches have been employed for developing ES and DSS for automatic ECG interpretation in heart abnormalities and disease diagnosis. They include knowledge-based, fuzzy, supervised learning, unsupervised learning, ensemble, neural-based, hybrid, and big data-based approaches.

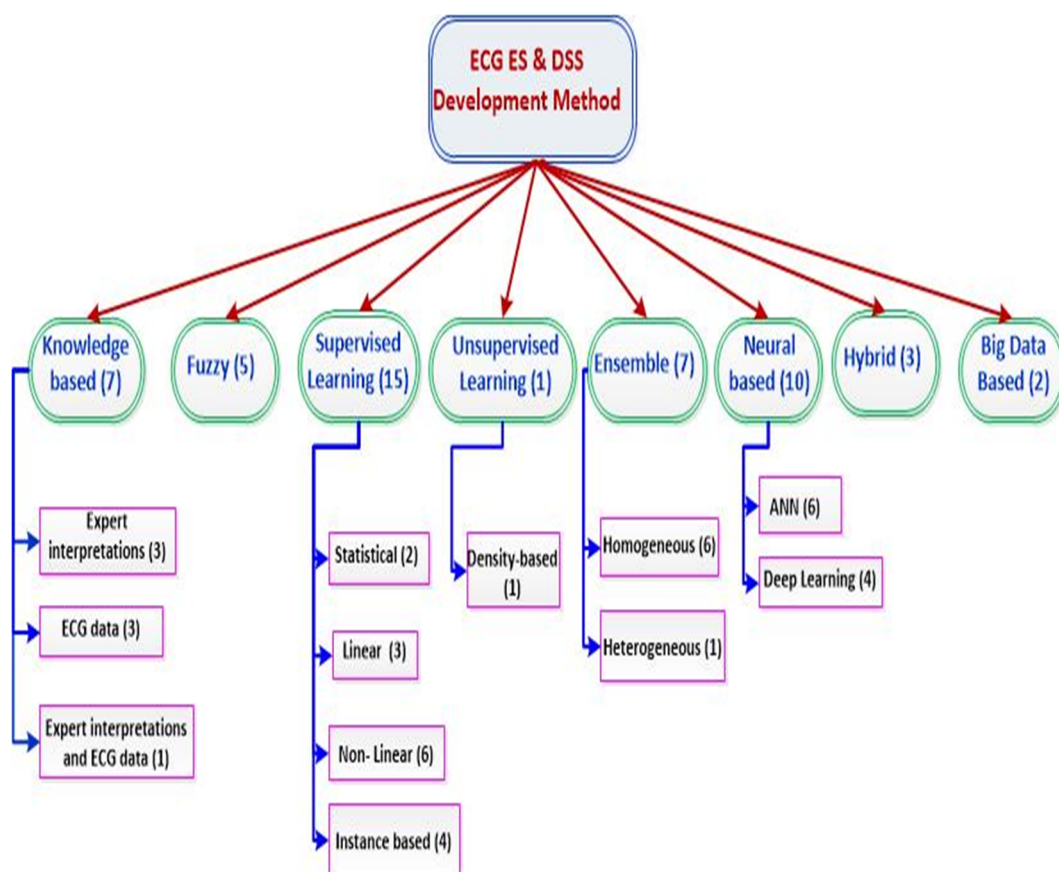


Figure 14. Taxonomy of Methods for ES/DSS Development in ECG Interpretation

This study identified fifty ~~(50)~~ works that proposed different methods for modelling, designing, and developing ES and DSS for automatic ECG interpretation. Knowledge-based approaches computationally represent expert knowledge using mathematical representations and design, whereas a rule-based system uses the represented knowledge for interpretation of ECG signals. Three methods were employed for building the knowledge base in this category in previous works; interpretations from

human experts, patient and ECG data collected, and the combination of the two. Fuzzy approaches interpret knowledge using fuzzy logic or fuzzy inference engine. Fuzzy approaches take a set of input data, fuzzify them, and apply some membership functions to the fuzzy set to predict the output. Fuzzy approach has witnessed some applications in ECG interpretation with about five works published. Supervised learning approach analyses a labeled set of inputs and generates a mapping between the input set and the output. It consists of regression and classification algorithms. Majorly, machine learning classification algorithms have been employed in most studies for the interpretation of ECG signals. We identified fifteen (15) works in this category that have been published in the last decade employing statistical, linear, non-linear, and instance-based classification methods. Notably, Support Vector Machine (SVM) has recorded more applications ~~and even more so~~ recently. Unsupervised learning approach explores an unlabeled set of input data and determines its underlying structure by generating clusters containing an input sets of similar characteristics. Unsupervised learning approach employs clustering and association rule mining algorithms. For the interpretation of ECG, we identified only one work that applied density-based clustering method. Ensemble approach combines one or more weak supervised learning approaches to build stronger learning model called metamodels. Ensemble methods (both homogenous and heterogenous) were applied in ~~about seven (7)~~ works for developing expert system and decision support systems in ECG interpretation as identified in our study.

Neural based approach (called neural network) is a type of machine learning approach that models the nervous system structure of the brain and how it works. The model is comprised of interconnected nodes organized into a connected network of neurons called neural network. Neurons in the neural networks are activated according to the data inputs (for example, ECG readings). Their activation propagates across the network to learn the relationship that maps the input data to the output data through a process called empirical learning [84]. The network is usually trained to optimize a specific cost function, which depends on the associated weights of the connections and data such as the sum-of-squares error or the cross-entropy [60]. This study identified ten ~~(10)~~ published works that employ artificial neural networks and deep neural network approaches in developing a robust ES/DSS for automatic ECG interpretation. Notably, current works in ECG interpretation are focusing on deep neural networks to handle the heterogenous big ECG signal data collected from IoT biosensors. Hybrid method integrate two different approaches to come up with a more powerful and efficient model for prediction. In the last decade, few works employed hybrid approaches for designing ES/DSS for ECG interpretation as our study recorded only three ~~(3)~~ published works in this category. Big data approaches, which employ robust methods called big data analytics for processing streams of large real-time data in a distributed cloud computing environment are recently applied in automatic ECG interpretation. This study was able to identify two ~~(2)~~ recently published works that **use** this approach. Figure 15 presents the proportion of methods in the published works identified in designing ES/DSS for ECG interpretation in the last decade. We also analyzed the trend in the rate of publications on ES/DSS development methods for ECG interpretation and diagnosis in the last decade from 2010 through 2020. The trend is presented in Figure 16.

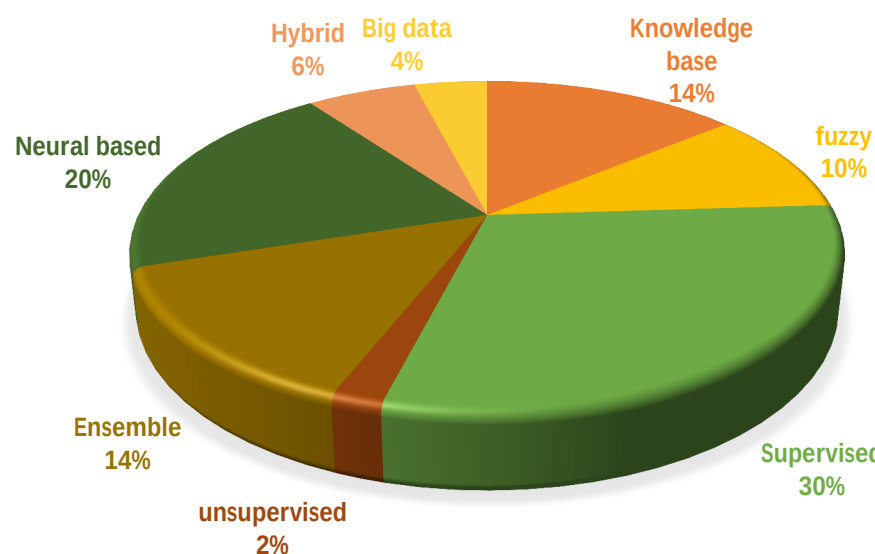


Figure 15. Percentage distribution of Methods for ES/DSS Development for ECG Interpretation

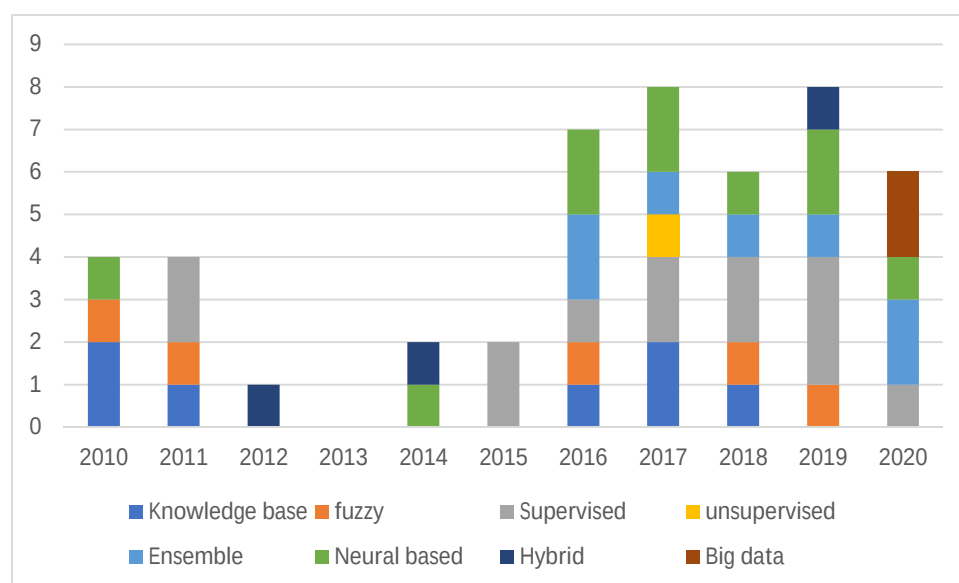


Figure 16. Trend in Publications on ES/DSS based ECG Interpretations in the Last Decade

An extensive review of works employing each of the identified methods is discussed in the following sections.

7.1 Knowledge-Based Approach

A considerable number of works in the expert systems for ECG interpretation focused on developing a knowledge base as a decision support for clinicians in differential diagnosis. Some of the works are based on collected ECG interpretations or rules from domain experts for building a knowledge base for ES. Bond, Finlay [31] proposed a rule-based markup language; ecgRuleML to make ECG rules interpretation accessible externally. EcgRuleML utilizes the eXtensible Markup Language (XML) to represent quantitative rules for measuring different cardiac parameters. To test the ecgRuleML model, rules were defined to assess ST Elevation Myocardial Infarction

(STEMI) in a Lux-192 Body Surface Potential Map (BSPM) based on a sample of 74 leads commonly used for STEMI assessment. Experimental evaluations showed that clinicians could use ecgRuleML to define new rules and update existing rules. Cloughley, Bond [57] built a knowledge base of thirty-eight (38) identified ECG diagnostic interpretations constructed from on-line ECG library databases. The knowledge base consists of characteristic data such as rhythm, wave, features, causes, sample images, and diagnostic report for each ECG recording. A query builder was built and connected to the knowledge base for the cardiologist to use as a decision support tool during the interpretation of ECG. The system, however, did not build a complete expert system to perform automatic interpretation but provided a very beneficial tool in assisting cardiologist in fast interpretation of ECG recordings. Similarly, Cairns, Bond [71] developed “Interactive Progressive-Based Interpretation” (IPI), an expert system based on Differential Diagnosis Algorithm (DDA) integrated with collected 375 human ECG interpretations to build a knowledge base for differential diagnosis. The system was modelled around the existing 12-lead ECG sensors. A rule-based reasoning algorithm was built to query the system. The IPI+DDA approach read 51.35% of the ECG readings correctly compared to the conventional approach with 42.61% correct interpretation of ECG readings.

Other works built the knowledge base from ECG and patient data collected from sensors and/or Electronic Health Records (EHR). Minutolo, Sannino [28] developed a rule-based decision support system for mobile cardiac heart monitoring using ontology. The system uses contextual information regarding the patient's posture and physical activities to detect and signal abnormal or emergency situations. The architecture of the proposed system is divided into three different layers, namely, Data Layer, Decisional Layer, and Action Layer. Data layer collects sensor data and represents them in the form of ontology description as a knowledge base. The Decision layer uses the ontology description and production rules to recognize all possible critical situations. Action layers executes the actions inferred by the Decision layer. The system or overall architecture was implemented in Java programming language and tested for effective performance. Similar approach was employed in Karvounis, Katertsidis [38] to develop an intelligent specialist decision support system for designing the best treatment plan for patients receiving Ventricular Assist Device (VAD) support before and after VAD implantation. The system works by analyzing patients' data to extract new knowledge and make intelligent decisions. Thai, Minh [4] presented a heart disease knowledge-based expert system built from a public heart disease dataset MIT-BIH Arrhythmia Database from Boston's Beth Israel Hospital for processing ECG signals from sensors to perform the diagnosis using a matching algorithm. Features were extracted using a combination of Sequential Recursive (SR), Discrete Wavelet Transform (DWT), and Fishers Linear Discriminant (FLD) algorithms. The proposed system was validated by a real data collected from human through ECG sensors and the results indicated the proposed model can perform a diagnosis that can support patients for pretreatment evaluation.

Recent works in knowledge-based approaches consider building a decision support system for collaborative diagnosis using both human expert interpretations and ECG data. Notable was the work of Wang, Sun [14] which presented an expert decision support system for collaborative diagnosis in remote cardiovascular healthcare by building an expert knowledge base and an auxiliary diagnosis expert decision support system on the basis of historical ECG diagnosis and treatment data. The approach is based on big data fusion and cloud computing. The proposed system was capable of supporting collaborative medicine, cooperative diagnosis and treatment.

7.2 Fuzzy-Based Methods

Some of the earliest works in expert systems for ECG interpretation employed fuzzy logic or fuzzy inference systems. Mahmoodabadi, Ahmadian [37] designed a fuzzy expert system to detect different types of arrhythmias from ECG signals. Wavelet signal analysis method using Daubechies wavelet family is used for signal analysis and ECG characteristic features extraction including P, Q, R, S, T waves, and the zero level of signal. Fuzzy rule-based classifier was used for 14 known arrhythmia type detections. Experimentation on MIT-BIH arrhythmia dataset gave a good results. However, the performance was low in some types of arrhythmia such as PVC and PAC. Abdullah, Zakaria [40] also designed a fuzzy expert system to predict the risk of hypertension in heart disease patients utilizing the fuzzy inference system (FIS) tool. The diagnosis was based on heart rate measured by ECG and other parameters such as blood pressure, BMI, and age. The approach performed better than other statistical approaches. In another study, Jeyalakshmi and Robin [61] developed an expert system for diagnosing sleep apnea from patient ECG recordings using fuzzy logic. The approach extracted HRV features from ECG signals which were fed into a fuzzy inference engine based on triangular membership function for diagnosis. The approach proved effective in detecting sleep apnea from patient ECG.

A recent study conducted by Jain and Kaur [82] presented a fuzzy expert system for the diagnosis of coronary artery disease using a rule base and membership functions based on different risk factors such as hypertension smoking, gender, age and family history. The expert system was developed in MATLAB and the proposed framework had 84.7% accuracy in the prediction of heart disease. The same approach was used in Sharma, Madaan [83] to develop an expert system for heart disease prediction using up to 19 risk features along with ECG recording. The system was able to predict low, middle, and high risk of heart disease in patients.

7.3 Supervised Learning Methods

Statistical supervised learning approach has earlier been used in developing expert system models for ECG interpretation and classification. de Oliveira, Andreão [41] employed Dynamic Bayesian Networks (DBN) to automatically detect heart arrhythmia (specifically PVC) in recorded long-term ECG. The expert system was tested on MIT-BIH arrhythmia dataset using the Bayesian Network Toolbox of MATLAB. Results indicated that DBN outperformed the static Bayesian Networks with a maximum accuracy of 98%. Quadratic Discrimination Analysis (QDA) was applied in Sterling, Huang [54] to develop a classification framework to predict Atrial Fibrillation (AF) recurrence in patients with direct-current electric (DCE) cardioversion from the underlying structure of ECG traces based on the matching pursuit (MP) feature extraction technique. The technique achieved 100% and 95% sensitivity and specificity, respectively, indicating the capability of the approach in providing reliable information for effective management of AF.

Some other studies considered linear and nonlinear supervised learning classifiers for automatic ECG interpretation. Alshraideh, Ootom [55] applied both linear (J48, Jrip, and ANN) and nonlinear (SVM) classifiers in building a web-based cardiovascular disease detection system that can identify different heart arrhythmias. The system used personal information of patients as input, together with several features extracted from the ECG signal analysis. The results showed that the highest classification accuracy was obtained by the linear classifiers, specifically J48, while nonlinear classifier (SVM) had poor performance. The same direction (applying both linear and nonlinear classifier) was followed by Khatibi and Rabinezhadsadatmahaleh [87] in developing automatic classification models for four types of arrhythmia using Decision Tree, SVM and RF.

However, the deep learning model CNN along with kNN approach were utilized for feature extraction after ECG signals were converted to image format. The approach proved very effective recording and better performance than SVM using polynomial kernel.

Instance-based supervised learning approach has also witnessed some applications in designing an expert systems for ECG interpretation. Desai, Martis [58] proposed a decision supportive ECG pattern recognition expert system using k-NN classifier based on Independent Component Analysis (ICA) with DWT feature extraction for five cardiac arrhythmia classes; Non-ectopic (N), Fusion (F), Ventricular ectopic (V), Supraventricular ectopic (S) and Unknown (U) beats. The approach was compared with SVM, ANN, and PNN based on different combinations of PCA and ICA with SVM, ANN, and PNN. The proposed approach applied on MIT-BIH Arrhythmia dataset outperformed the existing methods with an overall accuracy of 99.77%. k-NN has also been applied to DWT for noise removal, DCT for feature extraction, and PCA for dimensionality reduction by Desai [67] to detect coronary heart diseases from ECG signals collected from European databases. The approach outperformed SVM with an overall detection accuracy of 99.62. k-NN has also been applied by Goshvarpour and Goshvarpour [6] for developing expert system for ECG-based human identification using the fusion of characteristic features of ECG and Information theory indices extracted using Information Gain Ratio (IGR). The approach yielded a higher average accuracy rate of 97.62 ± 1.92 compared to the state-of-the-art approaches. In a current study, Kar, Sahu [93] employed k-NN based on Dual-Tree Complex Wavelet Transform for building heart beat arrhythmia classification decision support system using MIT-BIH Arrhythmia dataset. With the approach reaching an accuracy of 98.92%, it can be used effectively as a decision support system for detecting cardiac abnormalities.

SVM has seen more applications in the literatures compared to other supervised learning approaches for ECG analysis up till the present study. SVM was used by Kopiec and Martyna [39] for automatic ECG classification by analyzing 12-lead ECG waveforms. The analysis was done using the PTB Diagnostic ECG Database containing various instances of QRS complex, P-wave and T-wave morphologies. Empirical tests on 209 patients yielded a good result. Venkatesan, Karthigaikumar [18] proposed a Support Vector Machine (SVM)-based arrhythmic beat classification using ECG signal dataset from MIT-BIH to categorize patient heart status into normal and abnormal subjects. DWT along with DENLMS adaptive filter were used to extract HRV features from the ECG signals. Results from the experiments indicated that SVM based classifier achieved a maximum accuracy of 96 %. Linear SVM based on PCA Network (PCANet) feature extraction approach was also applied on MIT-BIH database ECG dataset for automatic recognition of five classes of arrhythmia by Yang, Si [17]. Their results indicated that the method has high recognition accuracy(up to 97.77%) in classifying noisy and skewed heartbeats. Jovic, Kukolja [86] presented a robust expert system platform for diagnosing arrhythmia from multivariate heterogenous medical time series consisting of ECG, EEG and HRV using SVM, MLP and NEAT. The approach tested on the dataset from MIT-BIH database yielded the highest accuracy of up to 77% on NEAT. The peculiarity of the system is that it can use any of the time series to perform the diagnosis. In another direction, Hejazi, Al-Haddad [65] applied One-Class SVM for building an ECG biometric authentication. The work built an authentication layer to provide the security of ECG recordings in a diagnostic expert systems.

7.4 Unsupervised Learning Methods

Application of unsupervised ML methods for ECG interpretation is very limited as few studies employed the clustering approach in designing underlying diagnostic

models for expert systems. This study could only find one work that employs clustering techniques within the expert system framework for ECG interpretation. Zhang, Wang [69] employed density-based clustering method to find representative beats as the training data for recurrent neural networks in classifying patient-specific ECG data.

7.5 Ensemble-Based Methods

Ensembles of supervised machine learning methods has also been applied in the development of expert decision support systems for ECG interpretation in previous studies. Alickovic and Subasi [34] designed a simple expert system for the detection and classification of arrhythmias based on Random Forest (RF) homogeneous ensemble classifier. DWT was employed for feature extraction by decomposing ECG signals into different successive frequency bands. Five most common arrhythmia beats types extracted from MIT-BIH and St.-Petersburg Institute of Cardiological Technics 12-lead Arrhythmia Databases were used. Results from the study showed that RF classifier resulted in better performance with a very high classification rate compared to other employed decision tree methods. RF in combination with Wavelet Packet Entropy (WPE) has also been used in Li and Zhou [123] for building high performance ECG signal interpretation model. The model yielded a promising result. Kumar, Pachori [77] also employed RF as the underlying model in the development of a decision support system for classification of permutation entropy (PEn) and log energy entropy (LEE), features extracted from 1000 ECG signals collected from MIT-BIH Atrial fibrillation (AF) database using flexible analytic wavelet transform (FAWT). The LEE feature with RF produced the highest accuracy of 96.84% in the prediction of AF. Recently, Christo, Nehemiah [89] proposed a clinical decision support system that employed RF with co-operative co-evolution feature selection method for automatic classification of various clinical datasets including Cleveland Heart Disease dataset (CHD) containing 303 instances with 13 features. The approach gave an effective diagnostic accuracy of 93% in heart disease prediction. Zarei and Asl [3] also reported better performance accuracy (93.26) for gentle-boost homogenous ensemble algorithm applied to automatically detect sleep apnea from ECG signals compared to other algorithms such as k-NN, SVM and ANN.

In some other studies, a heterogenous ensemble approach has also been employed. Yin and Jha [10] proposed ensemble methods for building a hierarchical expert clinical decision support system from physiological readings generated by Wearable Medical Sensors (WMS) for diagnosing various diseases. Their approach employed stacking, bagging, and boosting based on eight (8) different base classifiers. Results from experimentation indicated up to 86% diagnostic performance accuracy on arrhythmia. ~~The study estimated the storage capacity of building a clinical decision support systems for all known 69,000 human diseases to be 62GB in WMS tier.~~

7.6 Neural-Based Methods

Several configurations of neural networks have been employed for automatic prediction of various heart beat disorders based on ECG interpretation. Bellos, Papadopoulos [30] presented a rule-based expert system utilizing an artificial neural network model for predicting the severity of a health episodes in heart disease patients. The model made use of the fusion of ECG signals from wearable sensors and other measured patient parameters such as respiration, oxygen saturation (SpO₂), and temperature. The approach gave a competitive performance result although with low accuracy. Simple Artificial Neural Network (ANN) was also applied by Thomas, Das [53] for the classification of cardiac arrhythmias from ECG beats based on dual tree complex wavelet transform. The model evaluated on 12 files from MIT-BIH database yielded an overall accuracy of 97.8%. Li, Wang [59] applied General Regression Neural Network

(GRNN) to automatically classify personalized heart beats from long-term ECG recordings. Performance on 103 datasets yielded 95% accuracy. MLP neural network integrated with sample entropy and Fast Fourier Transform was used by Sadrawi, Lin [35] to automatically classify heart beat arrhythmia. The study in particular, evaluated four databases from PhysioNet consisting of AHADB, CUDB, MITDB, and NSTDB. The proposed integrated approach produced better accuracy under this setting than the state-of-the-art. Recently, Abdalla, Wu [33] applied a feed-forward ANN for automatic classification of five types of arrhythmia beats including NB, LBBB, APB, RBBB, and PVC. The technique was applied on Physionet MIT-BIH dataset based on Complete Ensemble Empirical Mode Decomposition with Adaptive Noise (CEEMDAN) for extracting linear features from the nonlinear ECG signal. Their approach was compared with the previous sixteen approaches and produced a better diagnostic accuracy of 99.9%. ANN was also explored by Parekh, Shah [91] for designing intelligent methods for fatigue detection based on EEG signals. Their findings revealed that the artificial neural networks can be used to recognize the alert and drowsy state of patients from ECG recordings.

Advanced neural networks with deep structures have also been utilized in recent works for ECG interpretation. As a step ahead, Ripoll, Wojdel [60] proposed a deep neural network with pretraining for automatic screening of patient ECG recordings for heart beat abnormalities. The pretraining was done with Restricted Boltzmann Machine (RBM) and the approach was tested through cross-validation on 416 test patients. Results from the evaluation indicated pretrained neural networks yielded an accuracy of 85.52% better than other networks without pretraining. This is due to the fact that neural networks with pretraining automatically generate a representation of the input data with no consideration for data annotation. Recurrent neural network, specifically LSTM, has also been applied by Zhang, Wang [69] to learn time correlation among ECG signal points for classifying ECG beats with different heart rates. The approach achieved state-of-the-art performance after evaluation on MIT-BIH dataset. Evolutionary neural system has also been applied for heart disease prediction based on ECG interpretation. Pławiak [76] employed evolutionary neural systems based on PNN, SVM, and RBFNN for automatic detection of myocardial dysfunction from 1000 fragments of ECG signals collected from the MIH-BIH Arrhythmia database for one lead and MLII from 45 patients. The Evolutionary system based on SVM produced the best result. In another work, a deep Two-Stage ANN with an adaptive filter approach was applied to measure fetal heart rate from mother surface ECG recordings by Kaleem and Kokate [85]. The approach was able to filter and detect the fetal signal marred by a pulse signal from the mother with a satisfying level of accuracy on 10 clinical cases from Physionet.

7.7 Hybrid Methods

As asserted by statistical studies carried out by Sahin, Tolun [44], earliest hybrid expert systems employed neuro-fuzzy and rough neural expert systems. Nevertheless, few hybrid expert system approaches have been presented in the literature for ECG interpretation and classification.

Acampora, Lee [42] proposed an ECG-based decision support system to deduce the cardiac condition of patients by hybridizing a Type-2 FML-based fuzzy inference machine with ontology to develop a knowledge-based fuzzy inference system. The system employed ontologies to improve the expressiveness of ECG knowledge base and Type-2 FML to model type-2 fuzzy systems. Empirical evaluation on 40 subjects revealed that the approach is feasible and can work effectively to infer the cardiac quality of patients. A hybrid framework based on kNN and a rule based system was proposed by Tanantong, Nantajeewarawat [52] for false alarm reduction in a continuous cardiac monitoring system using 3D acceleration ECG signal. k-nearest neighbor was employed

for constructing the model and rule-based expert system which consists of seven rules were constructed for false alarm detection. An accuracy of 96.7% with reduced false alarm rate was recorded based on validation on two datasets collected from the MIT-BIH arrhythmia database and 10 subjects conducting daily living activities (DLAs).

Recent work focused on hybrid deep learning approaches. Chauhan, Vig [81] presented a novel two-staged approach that combines a deep learning model with a supervised machine learning approach for anomaly detection and classification in ECG signals. In their work, LSTM, a recurrent deep neural network, was used for initial anomaly detection. In the first stage, LSTM was trained on large normal ECG patterns to identify the anomaly using prediction error. The error output was used in the second stage to predict the actual anomaly class in the pattern using Multi-Layer Perceptron (MLP), SVM, and Logistic Regression. Seven types of anomalies were investigated including Premature Ventricular Contraction (PVC), Atrial Premature Contraction (APC), pacing Beat (PB), Ventricular Bigeminy (VB), Ventricular Couplets (VCs), Ventricular Tachycardia (VT) and Right Bundle Branch Block (RBBB). Experimentation on MIT-BIH Arrhythmia dataset indicates that the proposed approach gave a promising result with the highest accuracy recorded by SVM (83.3%). This result indicates that the error vectors represented by their summary features carry useful predictive information about the actual ECG anomaly type.

7.8 Big Data-Based Methods

Current studies are focusing in the direction of designing a cloud-based big data framework for automatic and real-time interpretation of aggregated heterogeneous ECG signals from diverse sources. Big data analytics are employed to provide the processing capabilities to handle this large volume of data. Akhtar, Lee [88] presented state-of-the-art big data tools for dealing with multimodal data sources in the Intelligent Medical Platform (IMP) including ECG data. The IMP support data reader was used to provide a continuous real-time response for data analysis and visualization of multimodal data extracted from the nonvolatile storage based on queries from Apache Hive. To evaluate the performance of the IMP data acquisition and persistence platform, stress testing based on ECG signals was carried out with 500 data sources, as the number of devices increased incrementally several times. The results showed that the implementation, even with an increased number of devices, has been able to scale successfully. Similarly, Subasi, Bandic [90] proposed a cloud-based framework for fast real-time analysis of heterogeneous ECG and electroencephalogram (EEG) data streamed from smart biomedical sensors and smartphones. The framework was designed by combining the adaptive signal acquisition, segmentation, and denoising to optimize the signal transmission rate. Feature extraction was carried out using AR Burg model. Assessment of ECG and EEG signals was achieved by utilizing various machine learning algorithms. With this framework, the total computational power gained per class for the considered ECG and EEG signals are twice and four times better, respectively, than the classical approaches.

8. Challenges and Open Research Issues

In the last decade, there has been a lot of significant progress in the literature and industry towards the development of a robust ES and DSS for the interpretation and diagnosis of ECG traces. However, there are still some challenges and open research areas that need to be explored to improve on the state-of-the-art approaches. In this section, the identified challenges and open research areas that need concentration are highlighted based on the following categories:

- i. **Mobile App for ECG Interpretation:** At the acquisition step stands the mobile ECG App for collecting and preprocessing ECG traces directly from patients. The major challenge faced by this app is there the capability to acquire the full ECG data obtainable with 12-leads. Majority of the mobile apps in the market and the ones proposed in the literature are based on 1-6 leads which could not capture the complete electrophysiological events that occur in the heart. The limitation has affected the quality of interpretation and diagnosis made by ES systems that use such mobile apps. Novel approaches are needed to build mobile apps with the capability to acquire ECG data using 12-leads. Another major challenge is the security of the patient health data captured by the ECG mobile app. With the known sensitivity of the ECG data of patients and their intended privacy, the majority of the ECG apps do not consider securing the sensitive data from unauthorized access as it traverses the network. As an open research direction, mobile compliant encryption and steganography techniques are needed to ensure the security and privacy of the patients' data. Lastly, with the proliferation of mobile apps for the interpretation of ECG in the market, the majority of them are not validated. Effort is needed from the research community to carry out empirical validation of those apps in each other to ascertain their capabilities and reliability as well as proffer recommendations for their adoption.
- ii. **Feature Extraction for ECG interpretation:** Feature extraction is a major step in building ES or DSS for ECG interpretation that identifies salient characteristics from the ECG signals recorded for classification and interpretation. Due to the nonlinearity of the ECG signals, researchers in this area face some challenges in extracting characteristic features from the ECG. A major challenge in dealing with ECG is the existence of a lot of noise in the signal. Although different approaches have been proposed to reduce the effect of the existing noise within the ECG signals in the final interpretation, effective and applicable noise removal techniques are still required to clean the raw ECG signal before extraction. This is important to critically reduce, if not completely remove the classification error of the diagnostic ES built into the ECG signals. Another open research area that needs more concentration and focus is the error detection and correction from the ECG signals. As the recorded signals traverse the network, there is the possibility that the signal gets distorted or modified due to noise or transmission error. Therefore, the signal received by the feature extraction module might be dissimilar to the recorded ECG signal. Therefore, a robust error detection and correction technique such as hash function, checksum and cyclic redundancy check techniques can be introduced to further preprocess the signal before actual extraction. High dimensionality of the extracted features is another major problem encountered in building robust ES for ECG interpretation and diagnosis. It is a known fact that high data dimensionality affects the accuracy, speed of classification, and prediction algorithms. Majority of previous studies did not consider feature selection as a means to reduce the dimensionality of the extracted ECG features. Therefore, feature selection approaches such as filter, wrapper, embedded, and hybrid methods can be applied on ECG extracted features to reduce the high dimension, and in turn improve the efficiency and accuracy of the diagnostic ES for ECG interpretation.
- iii. **ECG Interpretation and Diagnostic Models:** Various approaches such as Knowledge-based, fuzzy-based, machine learning (majorly supervised), neural networks, ensemble, and hybrid approaches have been developed in the last decade to interpret the ECG traces and diagnose various abnormalities. Nevertheless, there is still room for improvement and extension of the current state-of-the-art approaches. Due to the complex structure of the ECG traces, especially the 12-led ECG, previously applied approaches have shown some limitations to correctly interpret the ECG data and diagnose multiple abnormalities. More studies are needed, especially in the

application of deep learning and hybrid deep learning techniques to correctly interpret the complex 12-lead ECG data and diagnose more abnormalities. Moreover, the number of samples/participants used for testing the developed diagnostic models in the existing studies are too small to generalize their effectiveness. More extensive testing methods are required to be carried out by new studies in ES development for ECG interpretation to confirm the reliability of the developed approaches in diagnosing heart abnormalities from ECG recordings. Another important challenge encountered in building classification models for ES in ECG interpretation is the class imbalance of the training dataset. Majority of the models in the existing studies used MIT-BIH Arrhythmia database for training which contains more percentage of normal than abnormal ECG. This class imbalance has been shown to cause overfitting. Although few studies tried to tackle this problem by applying ensemble methods, nevertheless, new studies in this area should consider deploying different techniques for class imbalance correction such as oversampling and undersampling to prevent classification overfitting which greatly affects the accuracy of the developed ES or DSS for ECG diagnosis. Another potential research area in this regard is the incorporation of other contextual information such as Body Mass Index (BMI), blood pressure, age, gender, and other similar parameters into ECG traces. This information could enhance the capability of the diagnostic models within the ES to accurately diagnose heart abnormalities.

- iv. **ES/DSS Development:** The ES/DSS is an application that provides real-time interpretation and diagnosis of abnormalities from the ECG recording of patients based on the underlying classification models. It has witnessed a series of developments in the last decade. However, majority of the developed systems are based on static knowledge. The ES/DSS applications for ECG interpretation and diagnosis can be improved upon in new studies by introducing an online/real-time update of ECG knowledge base to provide a more precise diagnosis. This can be achieved by carrying out system validation on an independent datasets for generalizability and a new patterns can be included in the knowledge base of ES system. Moreover, more studies should consider novel techniques for the fusion of ECG and other human biometrics for accurate identification and authorization of patients within the DSS system for ECG management.

9. Conclusion

ECG is one of the most widely used recordings in clinical medicine and several advancements in ECG tracing for diagnosing different diseases have been made over the past few years. The use of ECG recorded data for disease diagnosis has recently attracted large attention. Even though ECG signal is widely recorded in hospitals, it is also used in epidemiological studies as well as in large clinical trials. ES and DSS solutions have been developed to aid effective diagnosis of arrhythmias and other forms of abnormalities using ECG tracings. However, the literature lacks an extensive review of recent studies that may reveal growing areas for research advancement in this domain. Therefore, this paper presents an extensive review of studies that deal with the development of ES and DSS for ECG interpretation and diagnosis. Eighty-five (85) articles have been reviewed which spanned a period of a decade from 2010 to 2020 through a careful selection procedure guided by the PRISMA model. ES and DSS concepts, which guide the development of automated solutions for ECG recording towards diagnosing the patient's health condition have been discussed. This paper further presents a taxonomy of features and methods that have been adopted for developing efficient and effective ES and DSS solutions for ECG interpretation. Potential research questions to guide future research in this domain have also been highlighted.

Declarations:**Ethics approval and consent to participate**

All data originated from published articles.

Consent for publication

No individual person's data was presented.

Competing interests

No competing interests are reported by the authors

Data availability

The study is a review and no data required for the study

Acknowledgement

This research was supported by Princess Nourah bint Abdulrahman University Researchers Supporting Project number (PNURSP2022R178), Princess Nourah bint Abdulrahman University, Riyadh, Saudi Arabia

References

1. He, B. and R.J. Cohen, *Body surface Laplacian ECG mapping*. IEEE Transactions on Biomedical Engineering, 1992. **39**(11): p. 1179-1191.
2. Yakut, O., S. Solak, and E.D. Bolat. *Implementation of a web-based wireless ECG measuring and recording system*. in *17th International Conference on Medical Physics and Medical Sciences, Istanbul*. 2015.
3. Zarei, A. and B.M. Asl, *Automatic classification of apnea and normal subjects using new features extracted from HRV and ECG-derived respiration signals*. Biomedical Signal Processing and Control, 2020. **59**: p. 101927.
4. Thai, D.T., Q.T. Minh, and P.H. Phung. *Toward an IoT-based expert system for heart disease diagnosis*. 2017. CEUR Workshop Proceedings.
5. Zaorálek, L., *Classification of arrhythmia using machine learning techniques*. 2018.
6. Goshvarpour, A. and A. Goshvarpour, *Human identification using information theory-based indices of ECG characteristic points*. Expert Systems with Applications, 2019. **127**: p. 25-34.
7. Rautaharju, P. and H. Blackburn. *Relationship of blood pressure and ECG amplitudes and spatial vectors in healthy subjects*. in *Federation Proceedings*. 1960. Federation Amer Soc Exp Biol 9650 Rockville Pike, Bethesda, Md 20814-3998.
8. Pipberger, H.V., et al., *The electrocardiogram in epidemiologic investigations. A new classification system*. Circulation, 1982. **65**(7): p. 1456-1464.
9. Benharref, A., M.A. Serhani, and R. Mizouni. *Smart data synchronization in m-Health monitoring applications*. in *2014 IEEE 16th International Conference on e-Health Networking, Applications and Services (Healthcom)*. 2014. IEEE.
10. Yin, H. and N.K. Jha, *A health decision support system for disease diagnosis based on wearable medical sensors and machine learning ensembles*. IEEE Transactions on Multi-Scale Computing Systems, 2017. **3**(4): p. 228-241.
11. Vanathi, R. and A.S.A. Khadir. *A robust architectural framework for big data stream computing in personal healthcare real time analytics*. in *2017 World Congress on Computing and Communication Technologies (WCCCT)*. 2017. IEEE.
12. Mendis, S., et al., *World Health Organization definition of myocardial infarction: 2008–09 revision*. International journal of epidemiology, 2011. **40**(1): p. 139-146.
13. Laslett, L.J., et al., *The worldwide environment of cardiovascular disease: prevalence, diagnosis, therapy, and policy issues: a report from the American College of Cardiology*. Journal of the American College of Cardiology, 2012. **60**(25 Supplement): p. S1-S49.

- 1425 14. Wang, L., et al. *Multimode Data Fusion Based Remote Healthcare Framework*. in *Proceedings of the 2018 International Conference on*
1426 *Big Data Engineering and Technology*. 2018.
- 1427 15. WHO. *Cardiovascular Disease*. 2018 28th October 2019]; Available from:
1428 [http://www.who.int/news-room/fact-sheets/detail/cardiovascular-diseases-\(cvds\)](http://www.who.int/news-room/fact-sheets/detail/cardiovascular-diseases-(cvds)).
- 1429 16. Gahlot, S., S. Reddy, and D. Kumar, *Review of smart health monitoring approaches with survey analysis and proposed framework*.
1430 *IEEE Internet of Things Journal*, 2018. **6**(2): p. 2116-2127.
- 1431 17. Yang, W., et al., *Automatic recognition of arrhythmia based on principal component analysis network and linear support vector*
1432 *machine*. *Computers in biology and medicine*, 2018. **101**: p. 22-32.
- 1433 18. Venkatesan, C., et al., *ECG signal preprocessing and SVM classifier-based abnormality detection in remote healthcare applications*.
1434 *IEEE Access*, 2018. **6**: p. 9767-9773.
- 1435 19. Ford, F.N., *Decision support systems and expert systems: A comparison*. *Information & Management*, 1985. **8**(1): p. 21-26.
- 1436 20. Brucal, S., et al. *Portable electrocardiogram device using Android smartphone*. in *2016 38th Annual International Conference of the*
1437 *IEEE Engineering in Medicine and Biology Society (EMBC)*. 2016. IEEE.
- 1438 21. Li, K.H.C., et al., *The current state of mobile phone apps for monitoring heart rate, heart rate variability, and atrial fibrillation:*
1439 *narrative review*. *JMIR mHealth and uHealth*, 2019. **7**(2): p. e11606.
- 1440 22. Rong, G., et al., *Artificial Intelligence in Healthcare: Review and Prediction Case Studies*. Engineering, 2020.
- 1441 23. PRISMA. *Transparent Reporting of Systematic Reviews and Meta-Analyses*. 2020 2nd January 2020]; Available from:
1442 <http://www.prisma-statement.org/>.
- 1443 24. Stojmenski, A., M. Gusev, and I. Chorbev. *A mobile application for ECG detection and feature extraction*. in *Proceedings of the Int.*
1444 2016.
- 1445 25. Amour, N., et al., *Implementation of a mobile health system for monitoring ECG signals*, in *ASE*
1446 *BigData/SocialInformatics/PASSAT/BioMedCom 2014 Conference*. 2015: Harvard University.
- 1447 26. Domazet, E., M. Gusev, and L. Antovski. *Design specification of an ECG mobile application*. in *2017 25th Telecommunication*
1448 *Forum (TELFOR)*. 2017. IEEE.
- 1449 27. Bellos, C., et al. *Heterogeneous data fusion and intelligent techniques embedded in a mobile application for real-time chronic disease*
1450 *management*. in *2011 Annual International Conference of the IEEE Engineering in Medicine and Biology Society*. 2011. IEEE.
- 1451 28. Minutolo, A., et al. *A rule-based mHealth system for cardiac monitoring*. in *2010 IEEE EMBS Conference on Biomedical Engineering*
1452 *and Sciences (IECBES)*. 2010. IEEE.
- 1453 29. Sram, N. *An Ontology model-based ECG diagnostic solution*. in *2012 IEEE 13th International Symposium on Computational*
1454 *Intelligence and Informatics (CINTI)*. 2012. IEEE.
- 1455 30. Bellos, C.C., et al. *Extraction and Analysis of features acquired by wearable sensors network*. in *Proceedings of the 10th IEEE*
1456 *International Conference on Information Technology and Applications in Biomedicine*. 2010. IEEE.
- 1457 31. Bond, R.R., et al. *EcgRuleML: A rule-based Markup Language for describing diagnostic ECG criteria*. in *2010 Computing in*
1458 *Cardiology*. 2010. IEEE.
- 1459 32. Camara, C., et al., *Real-time electrocardiogram streams for continuous authentication*. *Applied Soft Computing*, 2018. **68**: p.
1460 784-794.
- 1461 33. Abdalla, F.Y., et al., *ECG arrhythmia classification using artificial intelligence and nonlinear and nonstationary decomposition*.
1462 *Signal, Image and Video Processing*, 2019. **13**(7): p. 1283-1291.
- 1463 34. Alickovic, E. and A. Subasi, *Medical decision support system for diagnosis of heart arrhythmia using DWT and random forests*
1464 *classifier*. *Journal of medical systems*, 2016. **40**(4): p. 108.
- 1465 35. Sadrawi, M., et al., *Arrhythmia evaluation in wearable ECG devices*. *Sensors*, 2017. **17**(11): p. 2445.

36. Catley, C., et al. *A framework to model and translate clinical rules to support complex real-time analysis of physiological and clinical data*. in *Proceedings of the 1st ACM International Health Informatics Symposium*. 2010.
37. Mahmoodabadi, S.Z., et al., *A fast expert system for electrocardiogram arrhythmia detection*. *Expert Systems*, 2010. **27**(3): p. 180-200.
38. Karvounis, E.C., et al. *An intelligent Decision Support System for the treatment of patients receiving Ventricular Assist Device (VAD) support*. in *2011 Annual International Conference of the IEEE Engineering in Medicine and Biology Society*. 2011. IEEE.
39. Kopiec, D. and J. Martyna. *A hybrid approach for ECG classification based on particle swarm optimization and support vector machine*. in *International Conference on Hybrid Artificial Intelligence Systems*. 2011. Springer.
40. Abdullah, A.A., Z. Zakaria, and N.F. Mohamad. *Design and development of fuzzy expert system for diagnosis of hypertension*. in *2011 Second International Conference on Intelligent Systems, Modelling and Simulation*. 2011. IEEE.
41. de Oliveira, L.S., R.V. Andreão, and M. Sarcinelli-Filho. *Premature ventricular beat classification using a dynamic Bayesian network*. in *2011 Annual International Conference of the IEEE Engineering in Medicine and Biology Society*. 2011. IEEE.
42. Acampora, G., et al., *Evaluating cardiac health through semantic soft computing techniques*. *Soft Computing*, 2012. **16**(7): p. 1165-1181.
43. Cinaglia, P., G. Tradigo, and P. Veltri. *A system for acquiring and management of ECG signals by using mobile devices: a support for first intervention in heart attacks*. in *Proceedings of the ACM Conference on Bioinformatics, Computational Biology and Biomedicine*. 2012.
44. Sahin, S., M.R. Tolun, and R. Hassanpour, *Hybrid expert systems: A survey of current approaches and applications*. *Expert systems with applications*, 2012. **39**(4): p. 4609-4617.
45. Paliwal, G. and A.W. Kiwelekar. *A comparison of mobile patient monitoring systems*. in *International Conference on Health Information Science*. 2013. Springer.
46. Belle, A., M.A. Kon, and K. Najarian, *Biomedical informatics for computer-aided decision support systems: a survey*. *The Scientific World Journal*, 2013. **2013**.
47. Lin, D., F. Labeau, and S. Mohapatra. *Decision support system for constantly monitoring patients in a comorbid condition*. in *2013 IEEE International Conference on Healthcare Informatics*. 2013. IEEE.
48. Prerana, N.G., A. Cheeran, and N.G. Sharma, *Android application for ambulant ecg monitoring*. *International Journal of Advanced Research in Computer and Communication Engineering*, 2014. **3**(5): p. 6465-6468.
49. Lin, D. and F. Labeau, *Monitoring Patients in a Comorbid Condition with the Aid of Computerized Decision Support System*, in *Concepts and Trends in Healthcare Information Systems*. 2014, Springer. p. 79-101.
50. Martínez-Pérez, B., et al., *Mobile clinical decision support systems and applications: a literature and commercial review*. *Journal of medical systems*, 2014. **38**(1): p. 4.
51. Sani, A.S., et al. *A framework for remote monitoring of early heart attack diagnosis system for ambulatory patient*. in *2014 IEEE Conference on Biomedical Engineering and Sciences (IECBES)*. 2014. IEEE.
52. Tanantong, T., E. Nantajeewarawat, and S. Thiemjarus. *False alarm reduction in continuous cardiac monitoring using 3D acceleration signals*. in *2014 International Computer Science and Engineering Conference (ICSEC)*. 2014. IEEE.
53. Thomas, M., M.K. Das, and S. Ari. *Classification of cardiac arrhythmias based on dual tree complex wavelet transform*. in *2014 international conference on communication and signal processing*. 2014. IEEE.
54. Sterling, M., D.T. Huang, and B. Ghoraani, *Developing a new computer-aided clinical decision support system for prediction of successful postcardioversion patients with persistent atrial fibrillation*. *Computational and Mathematical Methods in Medicine*, 2015. **2015**.
55. Alshraideh, H., et al., *A web based cardiovascular disease detection system*. *Journal of medical systems*, 2015. **39**(10): p. 122.

- 1507 56. Prakash, P., *Decision support system in heart disease diagnosis by case based recommendation*. Int. J. Sci. Technol. Res, 2015. **4**: p.
1508 51-55.
- 1509 57. Cloughley, R.G., et al. *An interactive clinician-friendly query builder for decision support during ECG interpretation*. in 2016
1510 *Computing in Cardiology Conference (CinC)*. 2016. IEEE.
- 1511 58. Desai, U., et al., *Decision support system for arrhythmia beats using ECG signals with DCT, DWT and EMD methods: a comparative*
1512 *study*. Journal of Mechanics in Medicine and Biology, 2016. **16**(01): p. 1640012.
- 1513 59. Li, P., et al., *High-performance personalized heartbeat classification model for long-term ECG signal*. IEEE Transactions on
1514 Biomedical Engineering, 2016. **64**(1): p. 78-86.
- 1515 60. Ripoll, V.J.R., et al., *ECG assessment based on neural networks with pretraining*. Applied Soft Computing, 2016. **49**: p. 399-406.
- 1516 61. Jeyalakshmi, M. and C. Robin, *Fuzzy based Expert system for sleep apnea diagnosis*. International Journal of Engineering Trends
1517 and Technology, 2016. **35**(12): p. 555-558.
- 1518 62. Kotevski, A., N. Koceska, and S. Koceski, *E-health monitoring system*. 2016.
- 1519 63. Baheti, M., *Study of need and framework of expert systems for medical diagnosis*. IOSR J Comput Eng.(IOSR-JCE) e-ISSN, 2016: p.
1520 2278-0661.
- 1521 64. Hassan, A.R. and M.I.H. Bhuiyan, *A decision support system for automatic sleep staging from EEG signals using tunable Q-factor*
1522 *wavelet transform and spectral features*. Journal of neuroscience methods, 2016. **271**: p. 107-118.
- 1523 65. Hejazi, M., et al., *ECG biometric authentication based on non-fiducial approach using kernel methods*. Digital Signal Processing,
1524 2016. **52**: p. 72-86.
- 1525 66. Gharehbaghi, A., M. Lindén, and A. Babic, *A decision support system for cardiac disease diagnosis based on machine learning*
1526 *methods*. Stud Health Technol Inform, 2017. **235**: p. 43-7.
- 1527 67. Desai, U. *Automated detection of cardiac health condition using linear techniques*. in 2017 2nd IEEE International Conference on
1528 *Recent Trends in Electronics, Information & Communication Technology (RTEICT)*. 2017. IEEE.
- 1529 68. Hassan, A.R. and M.A. Haque, *An expert system for automated identification of obstructive sleep apnea from single-lead ECG using*
1530 *random under sampling boosting*. Neurocomputing, 2017. **235**: p. 122-130.
- 1531 69. Zhang, C., et al. *Patient-specific ECG classification based on recurrent neural networks and clustering technique*. in 2017 13th
1532 *IASTED International Conference on Biomedical Engineering (BioMed)*. 2017. IEEE.
- 1533 70. Hossain, A., et al. *A crowd sourced framework for neighbour assisted medical emergency system*. in 2017 27th International
1534 *Telecommunication Networks and Applications Conference (ITNAC)*. 2017. IEEE.
- 1535 71. Cairns, A.W., et al., *A decision support system and rule-based algorithm to augment the human interpretation of the 12-lead*
1536 *electrocardiogram*. Journal of electrocardiology, 2017. **50**(6): p. 781-786.
- 1537 72. Krasteva, V., I. Jekova, and R. Abächerli, *Biometric verification by cross-correlation analysis of 12-lead ECG patterns: Ranking of*
1538 *the most reliable peripheral and chest leads*. Journal of electrocardiology, 2017. **50**(6): p. 847-854.
- 1539 73. Jung, W.-H. and S.-G. Lee, *ECG identification based on non-fiducial feature extraction using window removal method*. Applied
1540 Sciences, 2017. **7**(11): p. 1205.
- 1541 74. Hejazi, M., et al. *Non-fiducial based ECG biometric authentication using one-class support vector machine*. in 2017 *Signal Processing:*
1542 *Algorithms, Architectures, Arrangements, and Applications (SPA)*. 2017. IEEE.
- 1543 75. Jangra, P. and M. Gupta. *A Design of Real-Time Multilayered Smart Healthcare Monitoring Framework using IoT*. in 2018
1544 *International Conference on Intelligent and Advanced System (ICIAS)*. 2018. IEEE.
- 1545 76. Pławiak, P., *Novel methodology of cardiac health recognition based on ECG signals and evolutionary-neural system*. Expert Systems
1546 with Applications, 2018. **92**: p. 334-349.
- 1547 77. Kumar, M., R.B. Pachori, and U.R. Acharya, *Automated diagnosis of atrial fibrillation ECG signals using entropy features extracted*
1548 *from flexible analytic wavelet transform*. Biocybernetics and Biomedical Engineering, 2018. **38**(3): p. 564-573.

78. Arteaga-Falconi, J.S., H. Al Osman, and A. El Saddik, *ECG and fingerprint bimodal authentication*. Sustainable cities and society, 2018. **40**: p. 274-283.
79. Lee, S., et al., *Efficient fiducial point detection of ECG QRS complex based on polygonal approximation*. Sensors, 2018. **18**(12): p. 4502.
80. Comito, C., A. Forestiero, and G. Papuzzo. *A clinical decision support framework for automatic disease diagnoses*. in *Proceedings of the 2019 IEEE/ACM International Conference on Advances in Social Networks Analysis and Mining*. 2019.
81. Chauhan, S., L. Vig, and S. Ahmad, *ECG anomaly class identification using LSTM and error profile modeling*. Computers in biology and medicine, 2019. **109**: p. 14-21.
82. Jain, P. and A. Kaur. *A fuzzy expert system for coronary artery disease diagnosis*. in *Proceedings of the Third International Conference on Advanced Informatics for Computing Research*. 2019.
83. Sharma, S., et al. *Heart disease prediction using fuzzy system*. in *International Conference on Advanced Informatics for Computing Research*. 2018. Springer.
84. Mincholé, A. and B. Rodriguez, *Artificial intelligence for the electrocardiogram*. Nature medicine, 2019. **25**(1): p. 22-23.
85. Kaleem, A.M. and R.D. Kokate, *An efficient adaptive filter for fetal ECG extraction using neural network*. Journal of Intelligent Systems, 2019. **28**(4): p. 589-600.
86. Jovic, A., et al. *MULTISAB: A Web Platform for Analysis of Multivariate Heterogeneous Biomedical Time-series*. in *World Congress on Medical Physics and Biomedical Engineering 2018*. 2019. Springer.
87. Khatibi, T. and N. Rabinezhadsadatmahaleh, *Proposing feature engineering method based on deep learning and K-NNs for ECG beat classification and arrhythmia detection*. Australasian physical & engineering sciences in medicine, 2019: p. 1-20.
88. Akhtar, U., et al. *The Impact of Big Data In Healthcare Analytics*. in *2020 International Conference on Information Networking (ICOIN)*. 2020. IEEE.
89. Christo, V.E., et al., *Feature Selection and Instance Selection from Clinical Datasets Using Co-operative Co-evolution and Classification Using Random Forest*. IETE Journal of Research, 2020: p. 1-14.
90. Subasi, A., L. Bandic, and S.M. Qaisar, *Cloud-based health monitoring framework using smart sensors and smartphone*, in *Innovation in Health Informatics*. 2020, Elsevier. p. 217-243.
91. Parekh, V., D. Shah, and M. Shah, *Fatigue Detection Using Artificial Intelligence Framework*. Augmented Human Research, 2020. **5**(1): p. 5.
92. Santra, D., et al., *Rough set based lattice structure for knowledge representation in medical expert systems: low back pain management case study*. Expert Systems with Applications, 2020. **145**: p. 113084.
93. Kar, N., et al., *Effective ECG Beat Classification and Decision Support System Using Dual-Tree Complex Wavelet Transform*, in *Advances in Intelligent Computing and Communication*. 2020, Springer. p. 366-374.
94. Bhatt, A., S.K. Dubey, and A.K. Bhatt, *Proposed Model/Framework to Avoid Sudden Cardiac Arrest (SCA) and Sudden Cardiac Death (SCD) at Early Stage*, in *Soft Computing: Theories and Applications*. 2020, Springer. p. 683-694.
95. Hosseini, M.-P., et al., *Multimodal data analysis of epileptic EEG and rs-fMRI via deep learning and edge computing*. Artificial Intelligence in Medicine, 2020. **104**: p. 101813.
96. Raheja, N. and A.K. Manocha, *A Study of Telecardiology-Based Methods for Detection of Cardiovascular Diseases*, in *Recent Trends in Image and Signal Processing in Computer Vision*. 2020, Springer. p. 165-179.
97. Maji, U., et al., *An IoT-Based Remote Health Monitoring System for Smart Healthcare: Cardiac Health Monitoring-Based Approach*, in *Advancements in Instrumentation and Control in Applied System Applications*. 2020, IGI Global. p. 231-254.
98. Dilaveris, P.E., et al., *Simple electrocardiographic markers for the prediction of paroxysmal idiopathic atrial fibrillation*. American heart journal, 1998. **135**(5): p. 733-738.

99. Elgendi, M., et al., *Revisiting QRS detection methodologies for portable, wearable, battery-operated, and wireless ECG systems*. PloS one, 2014. **9**(1).
100. Hasan, M. and M. Mamun, *Hardware approach of R-peak detection for the measurement of fetal and maternal heart rates*. Journal of applied research and technology, 2012. **10**(6): p. 835-844.
101. Thong, T., et al. *Paroxysmal atrial fibrillation prediction using isolated premature atrial events and paroxysmal atrial tachycardia*. in *Proceedings of the 25th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (IEEE Cat. No. 03CH37439)*. 2003. IEEE.
102. Tsipouras, M.G., D.I. Fotiadis, and D. Sideris. *Arrhythmia classification using the RR-interval duration signal*. in *Computers in cardiology*. 2002. IEEE.
103. Trinder, J., et al., *Autonomic activity during human sleep as a function of time and sleep stage*. Journal of sleep research, 2001. **10**(4): p. 253-264.
104. Benitez, D., et al., *The use of the Hilbert transform in ECG signal analysis*. Computers in biology and medicine, 2001. **31**(5): p. 399-406.
105. Burte, R. and R. Ghongade, *Advances in QRS detection: Modified Wavelet energy gradient method*. International Journal of Emerging Trends in Signal Processing, 2012. **1**(1): p. 23-29.
106. Tan, C., et al., *The application of expert system: A review of research and applications*. ARPN Journal of Engineering and Applied Sciences, 2016. **11**(4): p. 2448-2453.
107. Akram, M., I.A. Rahman, and I. Memon, *A review on expert system and its applications in civil engineering*. International Journal of Civil Engineering and Built Environment, 2014. **1**(1): p. 24-29.
108. Nagori, V. and B. Trivedi, *Types of expert system: comparative study*. Asian Journal of Computer and Information Systems (ISSN: 2321-5658), 2014. **2**(02).
109. Pambudi Utomo, T. and N. Nuryani. *QRS peak detection for heart rate monitoring on Android smartphone*. in *Journal of Physics Conference Series*. 2017.
110. Teja, A.D. and K.S. Rao, *A Smart Wearable System for ECG and Health Monitoring*. International Journal for Advance Research and Development, 2018. **3**(2): p. 57-63.
111. Marshall, I. and J. Neilson, *Mains interference in ECG recording*. Journal of medical engineering & technology, 1984. **8**(4): p. 177-180.
112. Rahman, M.Z.U., R.A. Shaik, and D.R.K. Reddy, *Efficient and simplified adaptive noise cancelers for ECG sensor based remote health monitoring*. IEEE Sensors Journal, 2011. **12**(3): p. 566-573.
113. Benesty, J., Y.A. Huang, and J. Chen, *Wiener and adaptive filters*, in *Springer Handbook of Speech Processing*. 2008, Springer. p. 103-120.
114. Israel, S.A., et al., *ECG to identify individuals*. Pattern recognition, 2005. **38**(1): p. 133-142.
115. Biel, L., et al., *ECG analysis: a new approach in human identification*. IEEE Transactions on Instrumentation and Measurement, 2001. **50**(3): p. 808-812.
116. Odinaka, I., et al., *ECG biometric recognition: A comparative analysis*. IEEE Transactions on Information Forensics and Security, 2012. **7**(6): p. 1812-1824.
117. Chan, A.D., et al., *Wavelet distance measure for person identification using electrocardiograms*. IEEE transactions on instrumentation and measurement, 2008. **57**(2): p. 248-253.
118. Chiu, C.-C., C.-M. Chuang, and C.-Y. Hsu. *A novel personal identity verification approach using a discrete wavelet transform of the ECG signal*. in *2008 International Conference on Multimedia and Ubiquitous Engineering (mue 2008)*. 2008. IEEE.
119. Banu, U. and G. Patil, *A survey on automatic ECG analyzing system*. Indian Journal of Scientific Research, 2015: p. 246-252.

-
- 1631 120. Anto, S., S. Chandramathi, and B. Femina, *An Expert System based on SVM and Hybrid GA-SA Optimization for Disease*
1632 *Diagnosis*. International Journal of Biology and Biomedicine, 2017. **2**.
- 1633 121. Kaur, G. and P. Kaur, *A Review on Fuzzy Rule Based Expert System To Diagnose Human Diseases*. 2017.
- 1634 122. Golubovski, R. and G. Markoski, *Expert System Application in Support of Automated ECG Diagnosis*. Balkan Journal of Applied
1635 Mathematics and Informatics, 2019. **2**(1): p. 29-38.
- 1636 123. Li, T. and M. Zhou, *ECG classification using wavelet packet entropy and random forests*. Entropy, 2016. **18**(8): p. 285.
- 1637